

IMBL: X-ray characteristics & general imaging




Andrew Stevenson
IMBL, Australian Synchrotron
& CSIRO Manufacturing



CT@IMBL workshop – 20th March, 2017

The “first” X-ray image

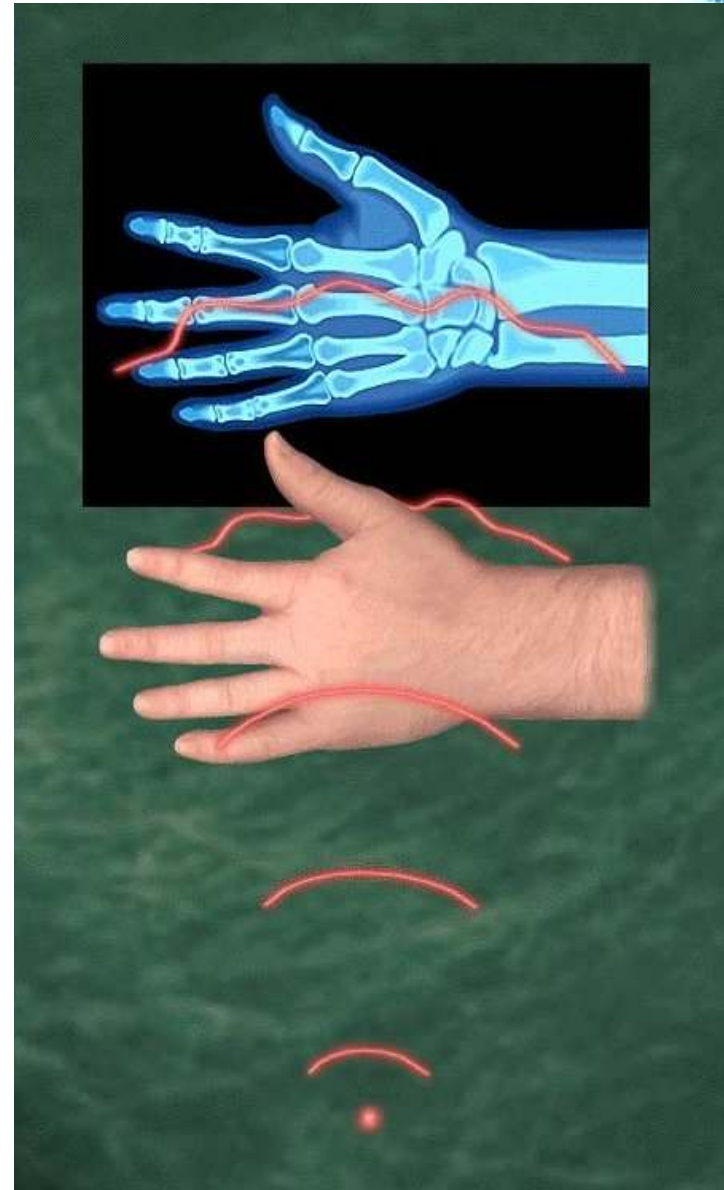


basic assumptions of conventional radiography




- 1. Contrast is produced purely by absorption in the object.**
- 2. Ray (or geometrical) optics is sufficient to describe image structure.**
- 3. It is not (usually) necessary to attempt to extract quantitative information from images.**

laboratory-based PCX imaging system

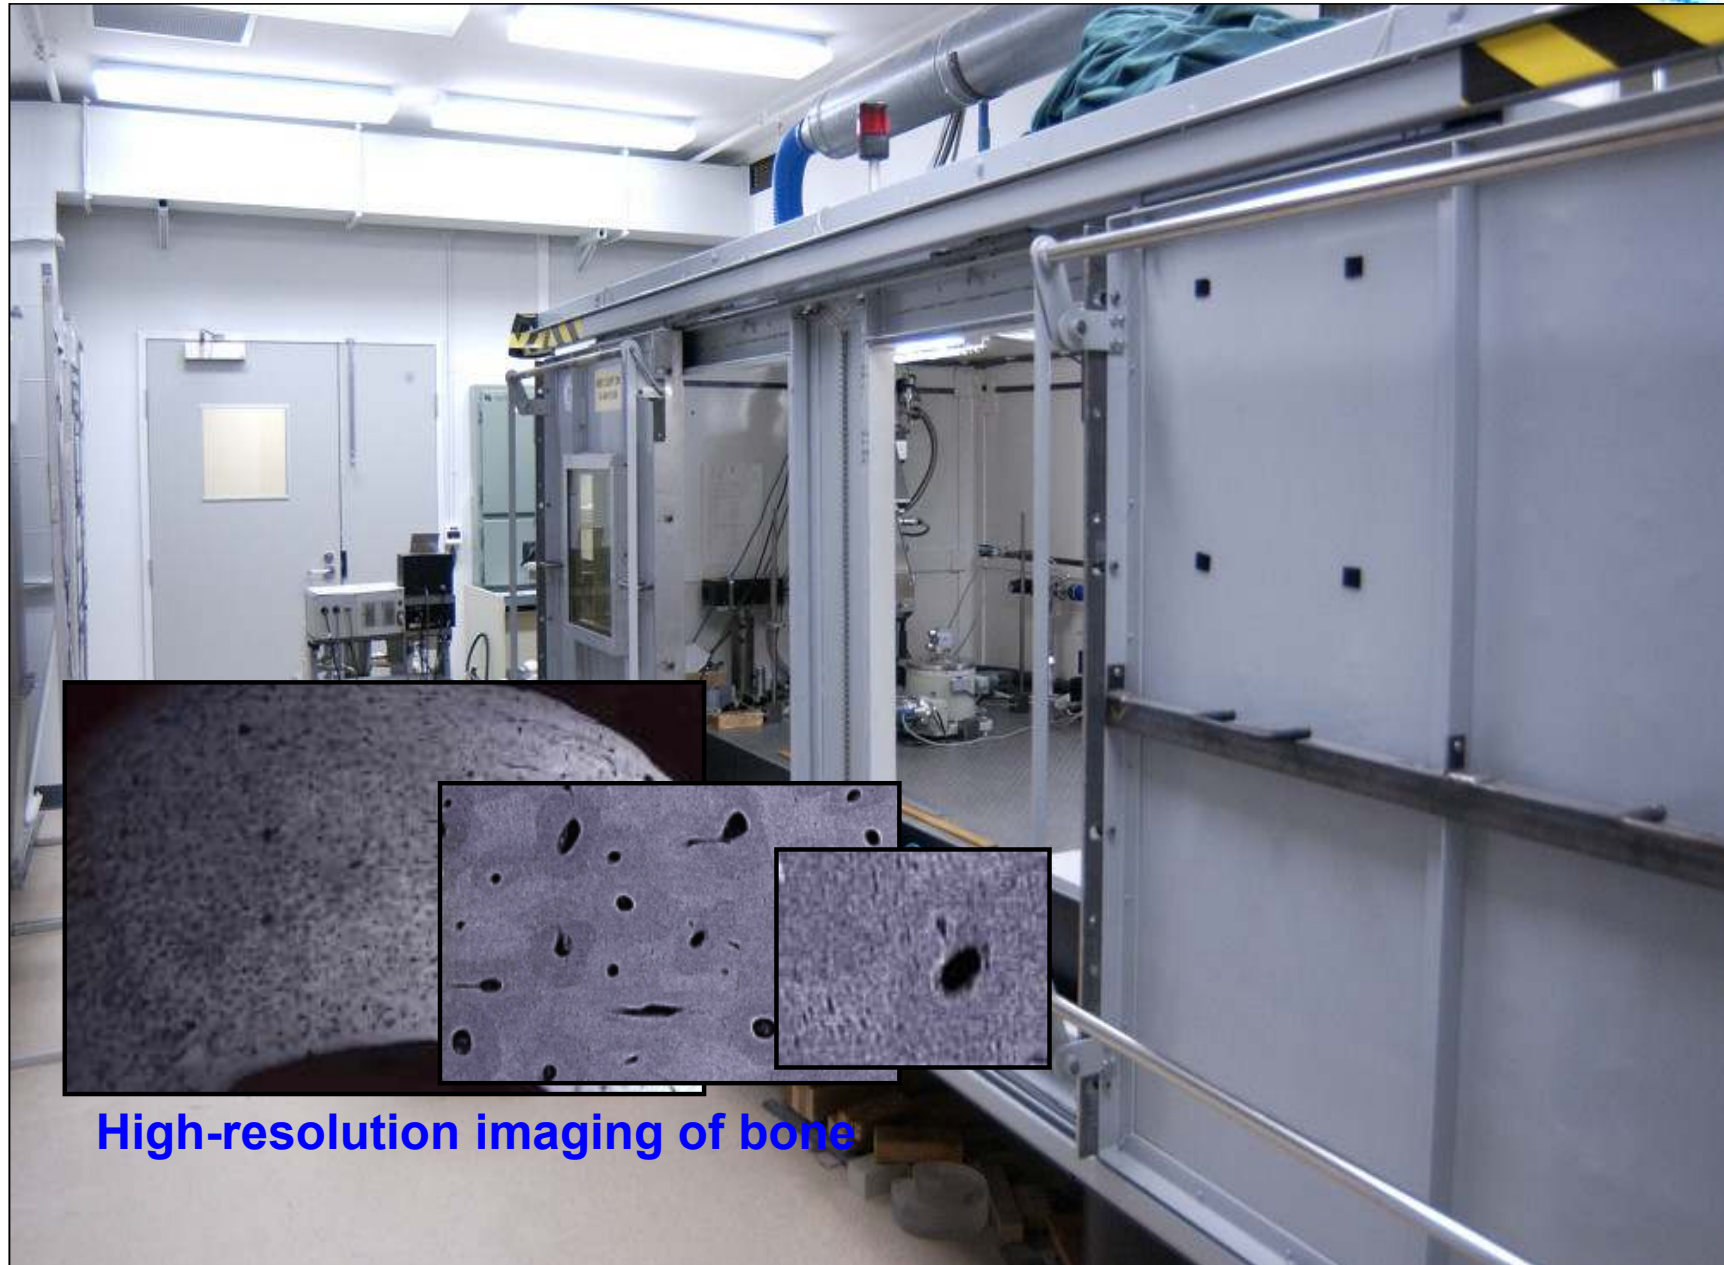


High-resolution imaging of bone


Feinfocus microfocus X-ray source - imaging and microtomography

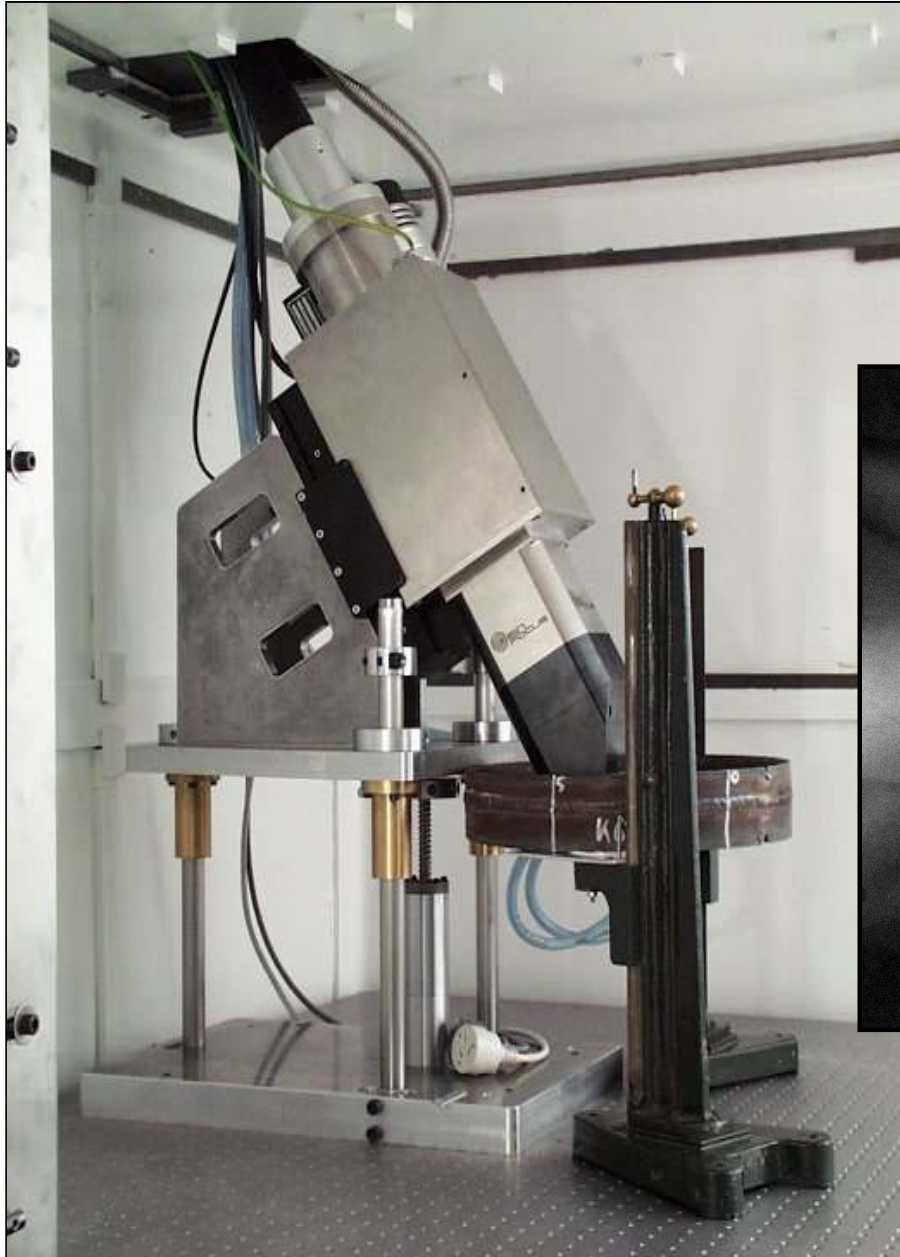

**hot tear in girth weld for
9mm steel pressure pipe**

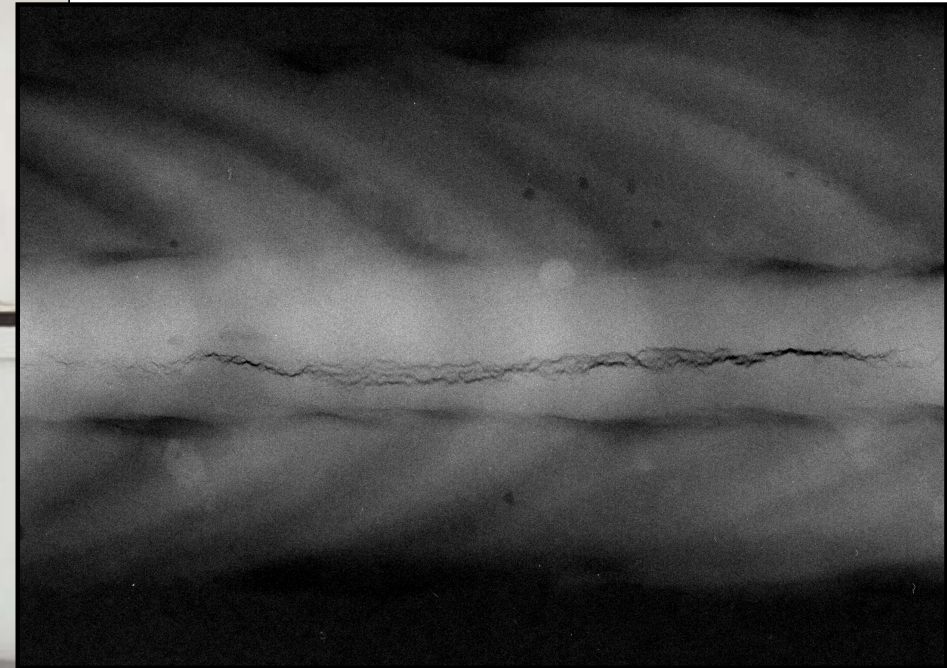

human finger (proximal phalanx)


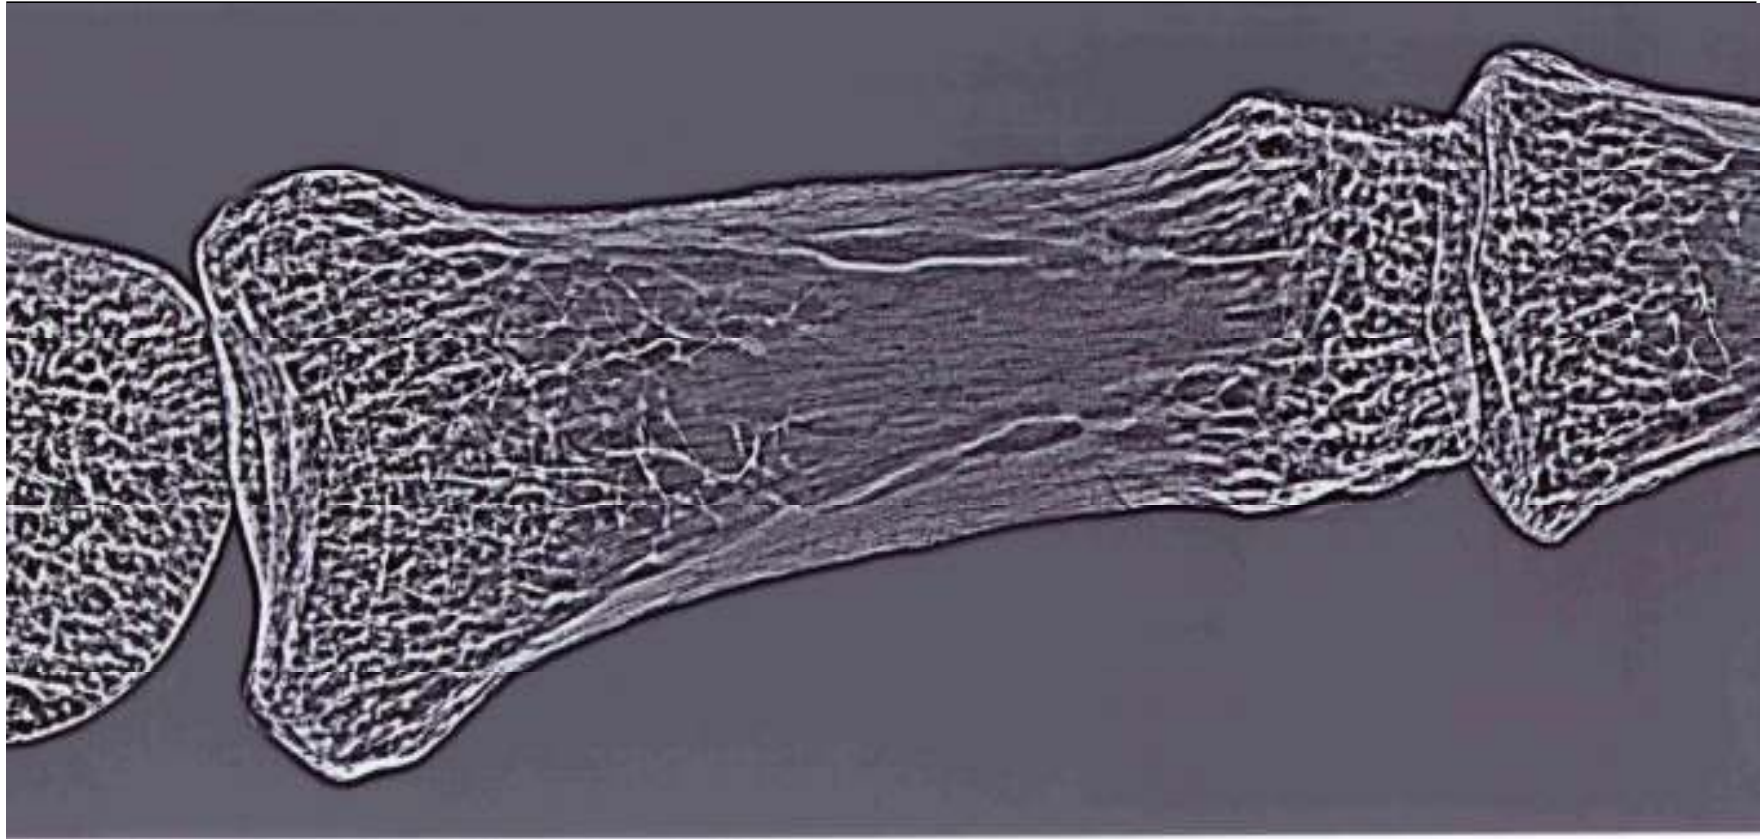


“unsharp masking”


excised mouse kidney




cochlear implant

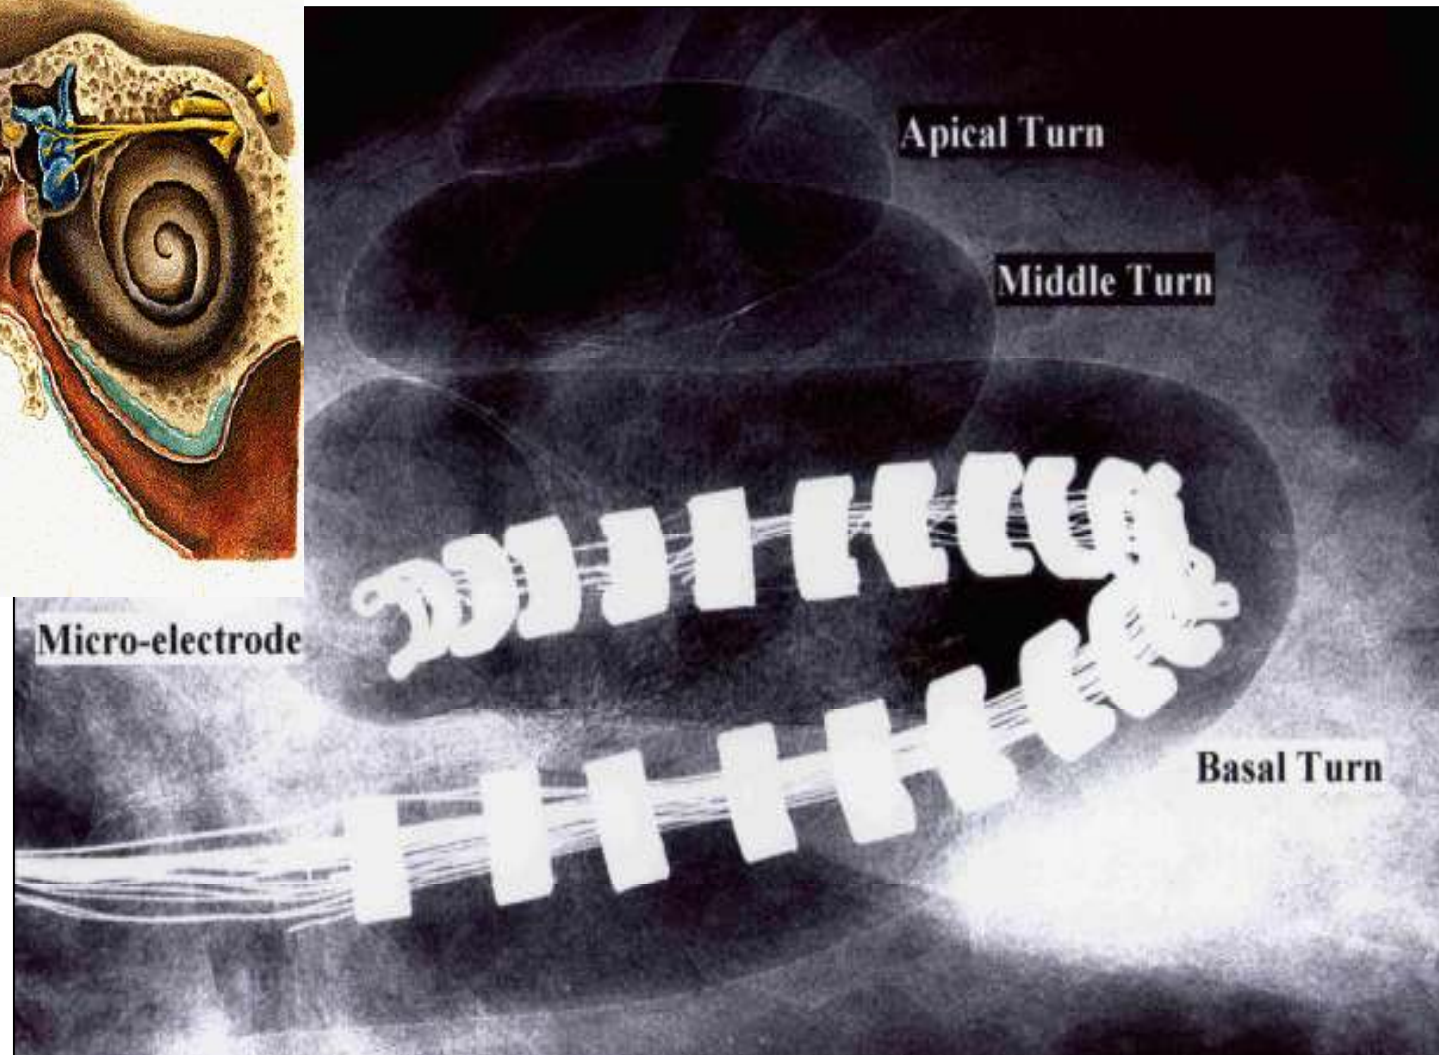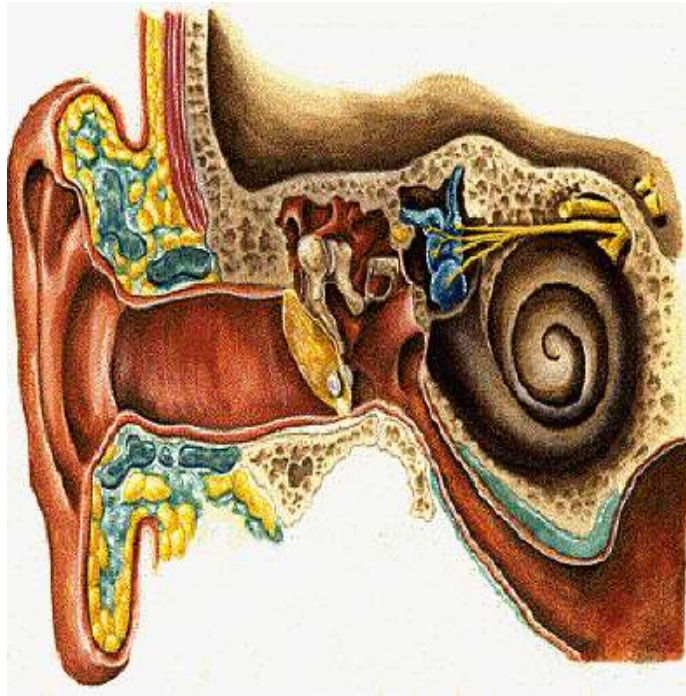



thin wood cross-section

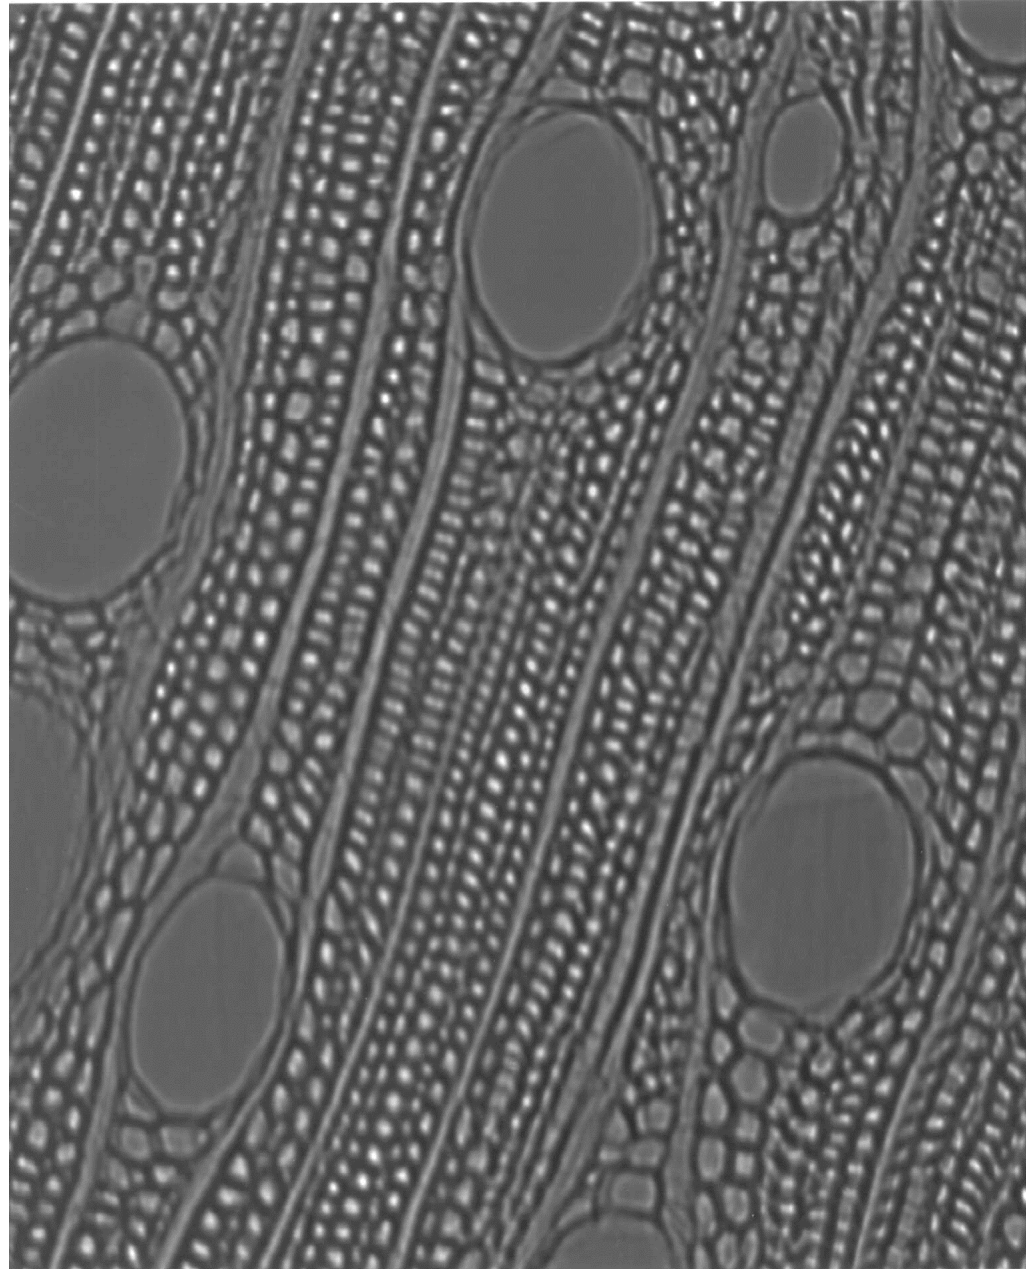


mouse tibia - X-ray tomography

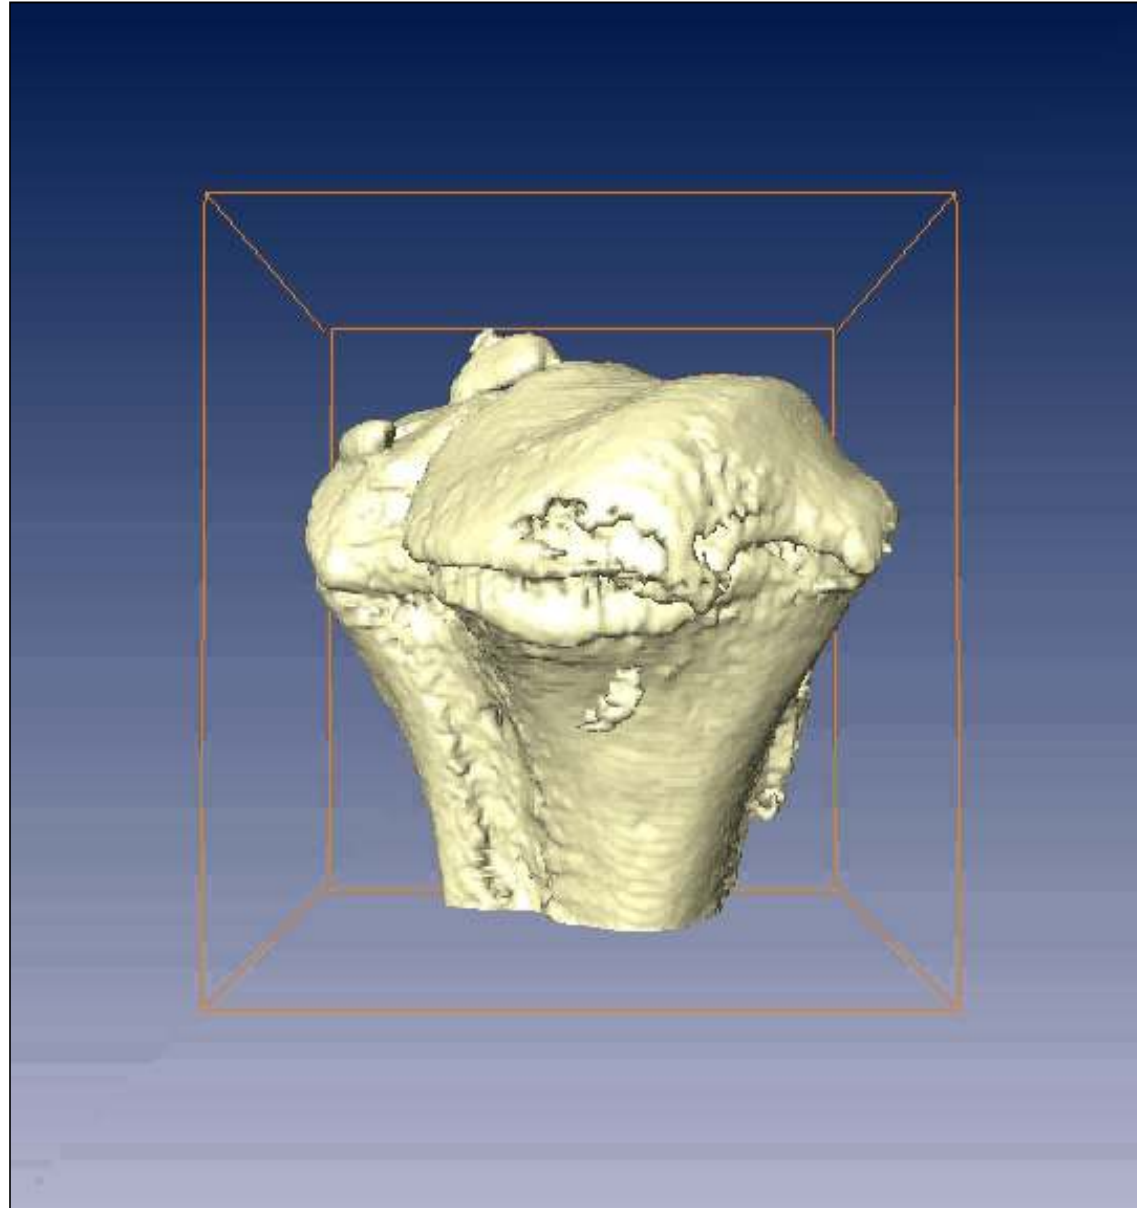

X-ray tomography on fixed & embedded rat brains

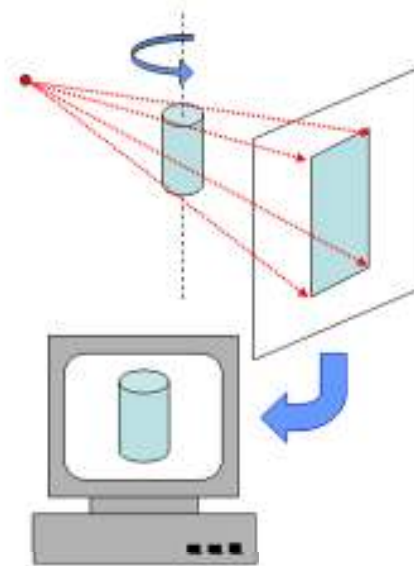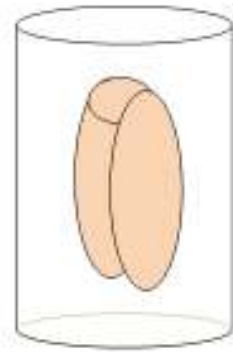

Imaging and Medical Beamline (IMBL)

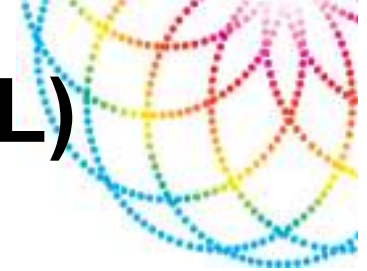


Monash Biomedical Imaging (MBI)
– Monash/CSIRO

IMBL end station
at 140m

transfer tunnel




**~140m - mode 3: high-resolution
imaging (incl PCI) & (slower) CT**

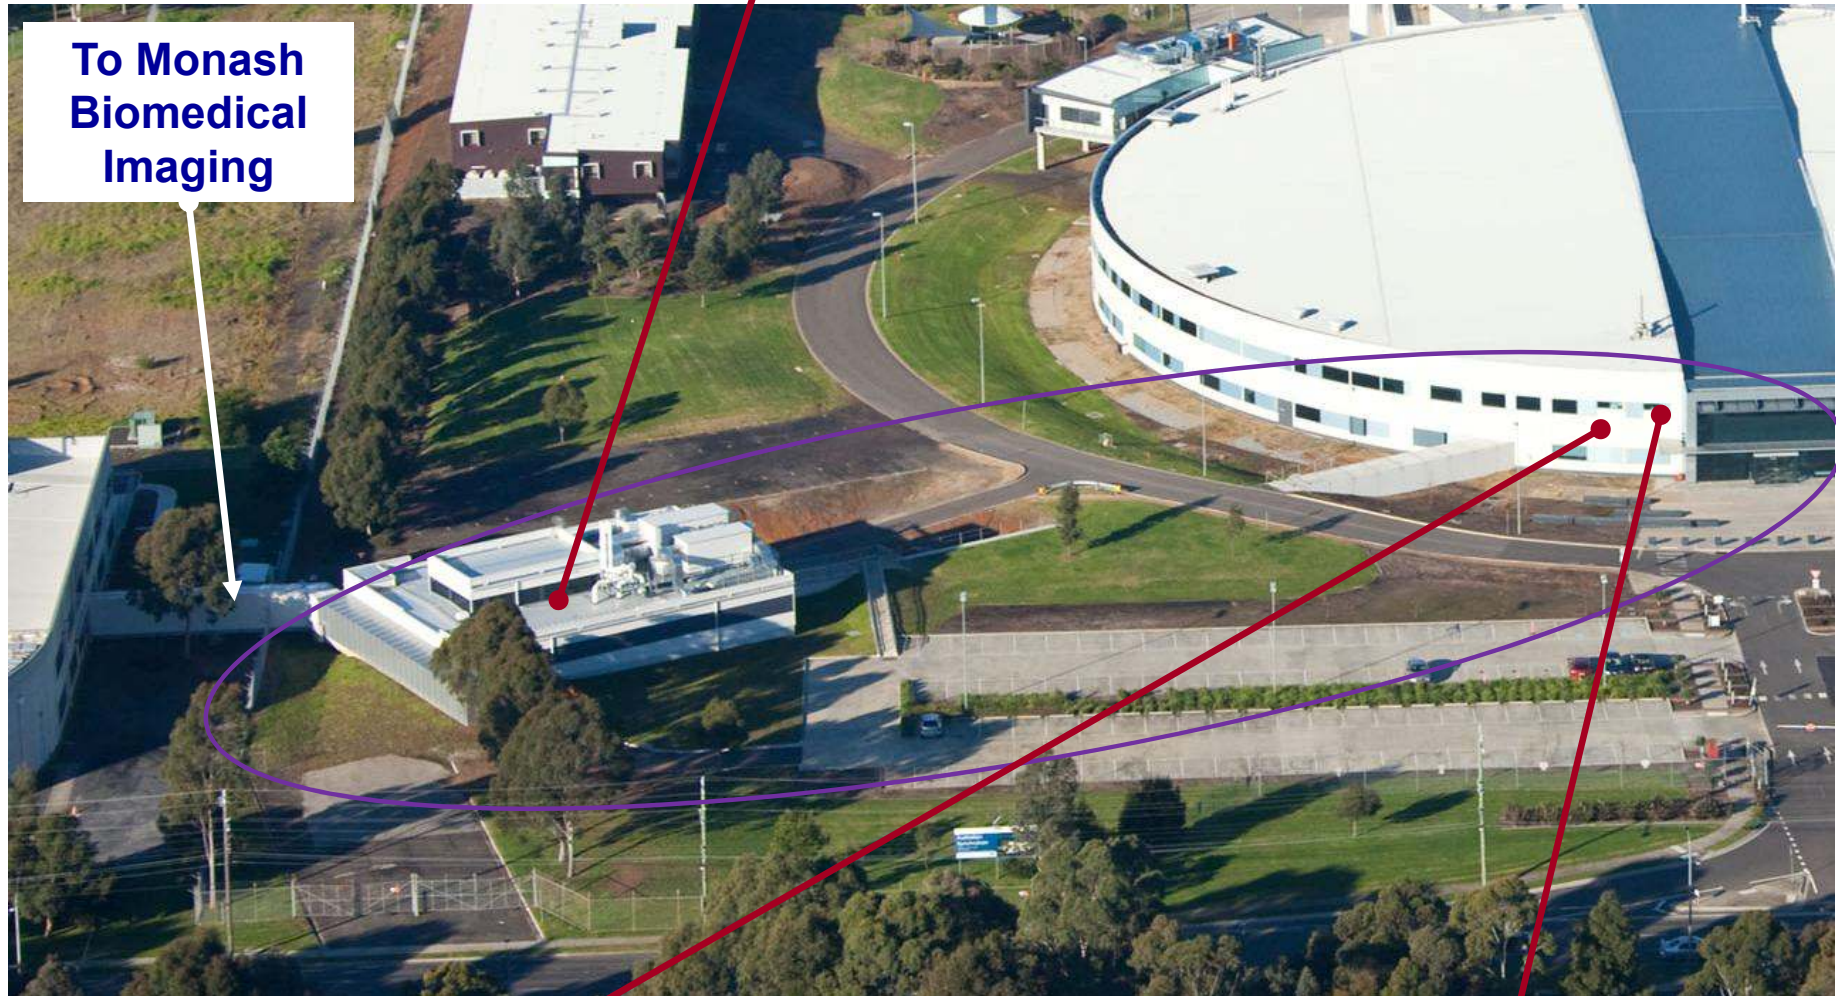



**To Monash
Biomedical
Imaging**


**~36m – mode 2: fast imaging &
CT, lower-dose radiotherapy**

**~22m - mode 1: high-
dose radiotherapy**

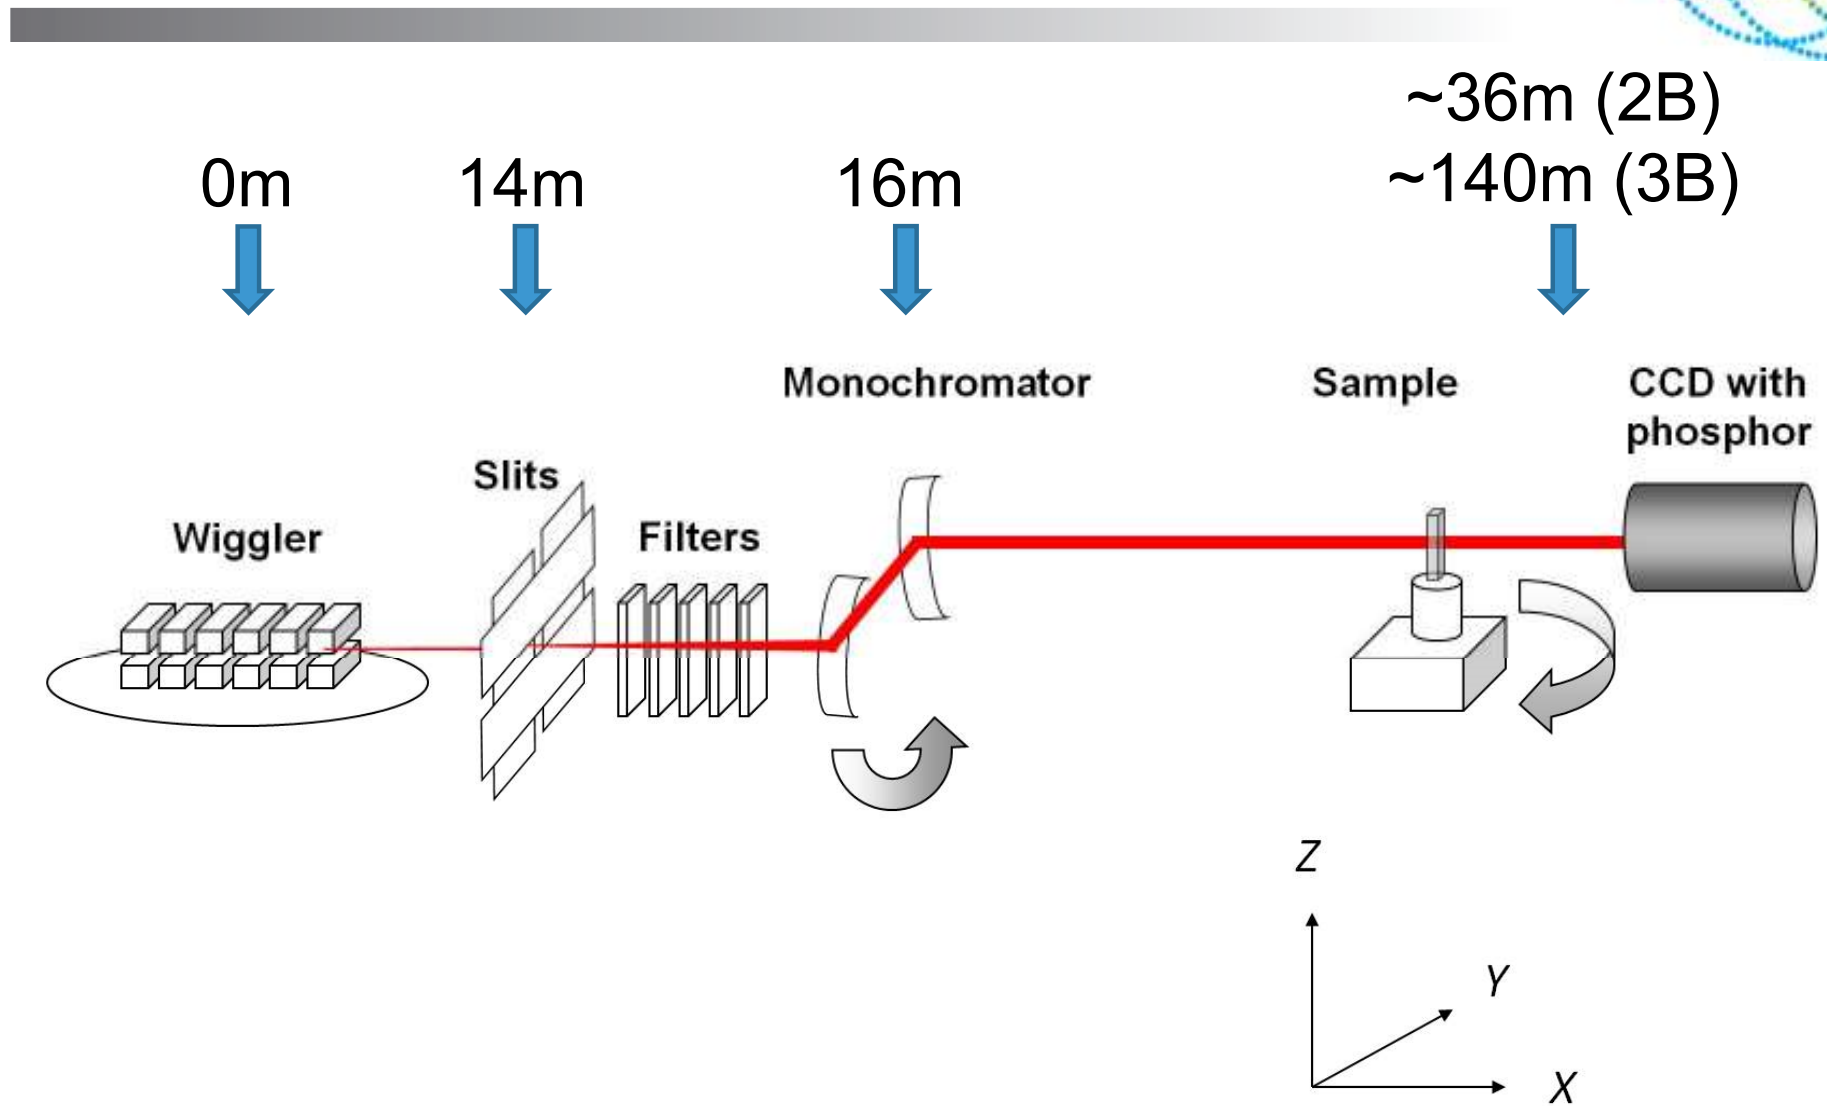

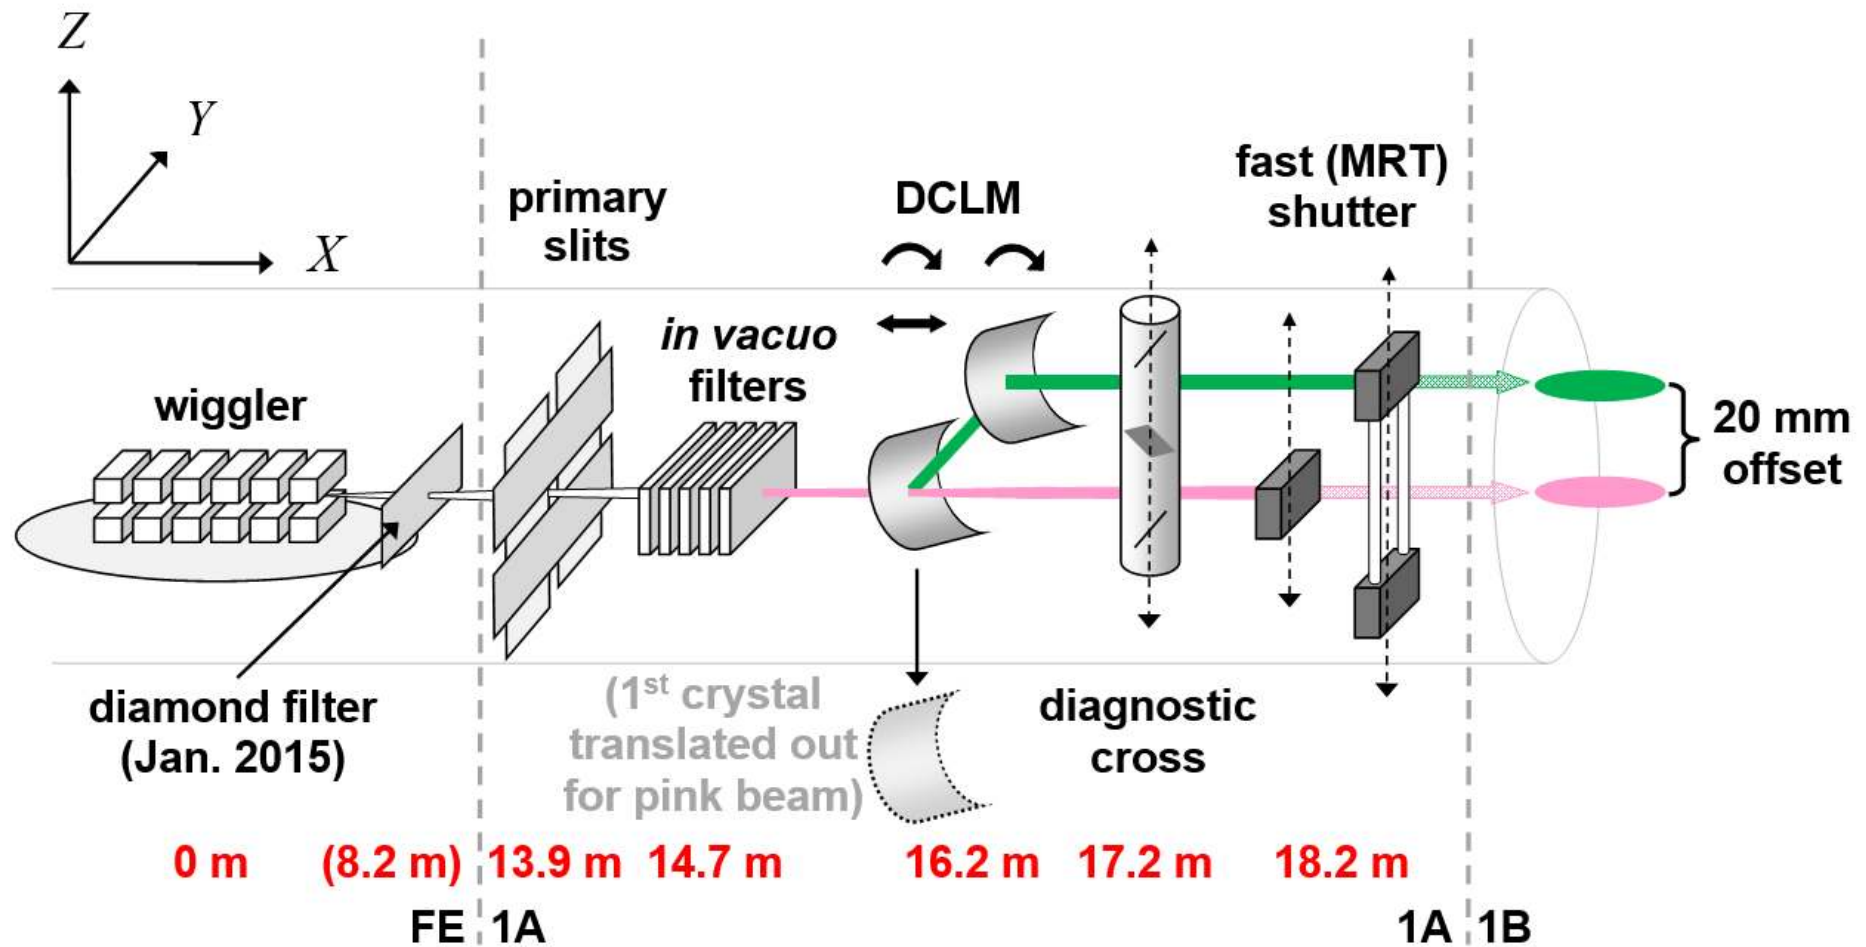


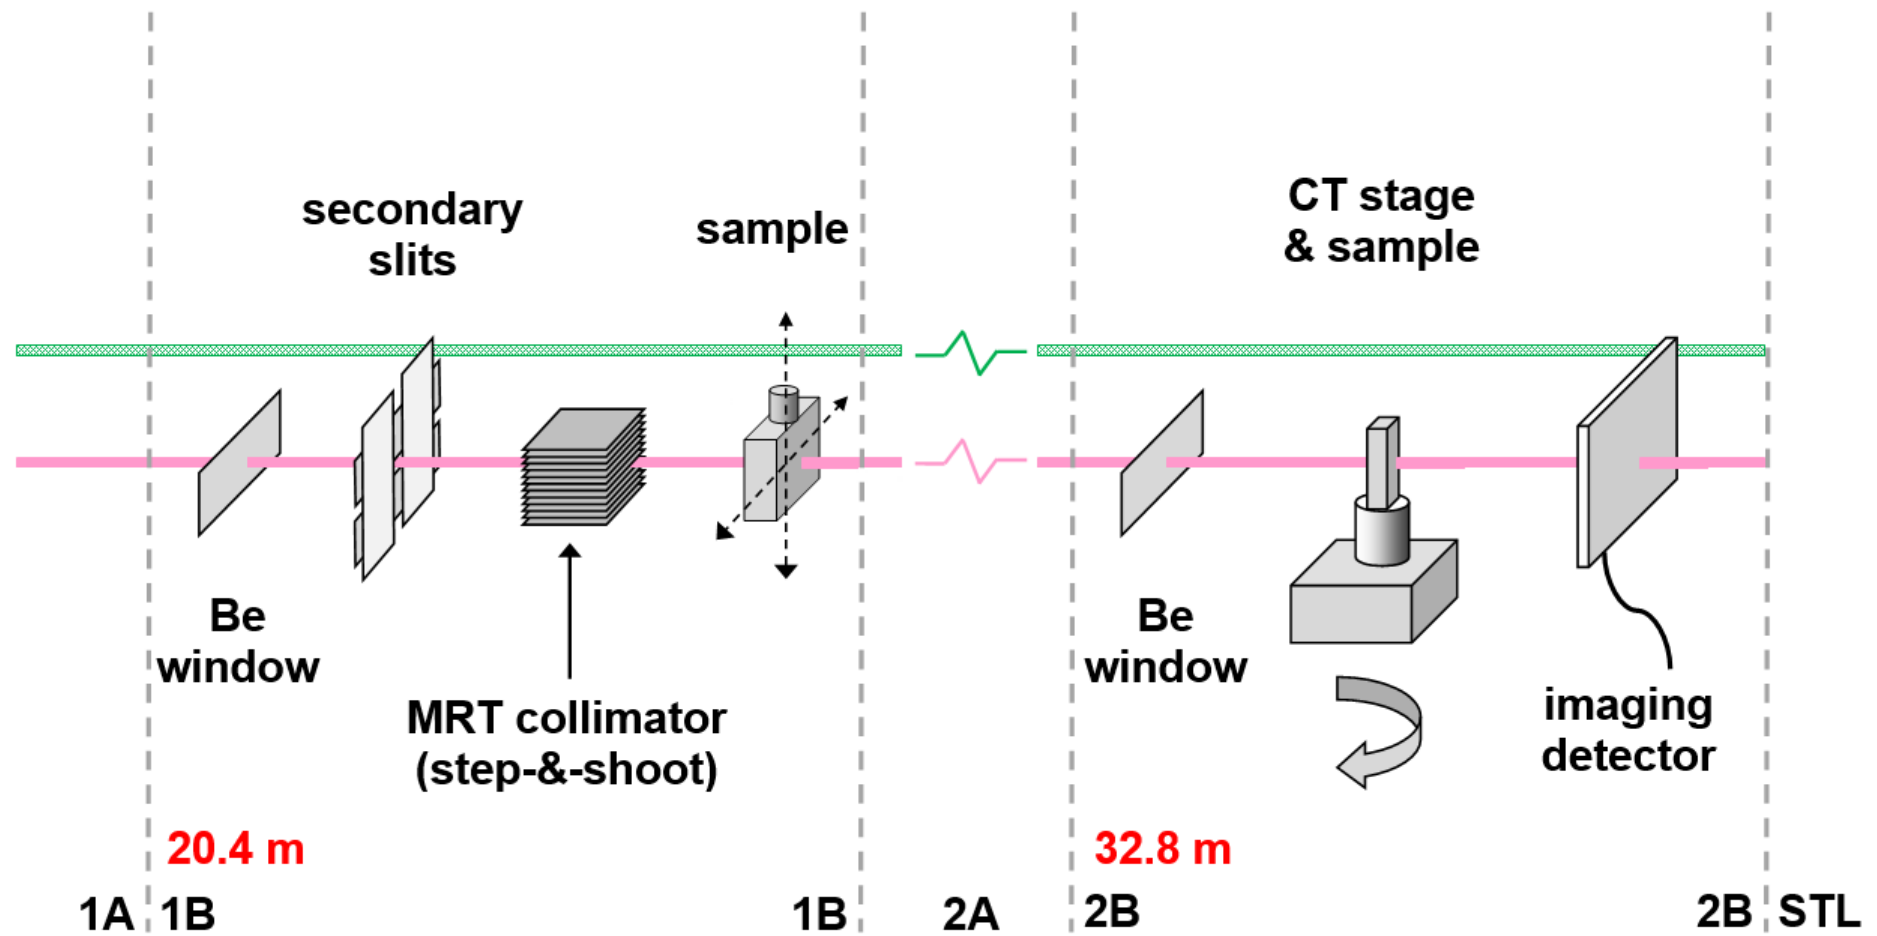


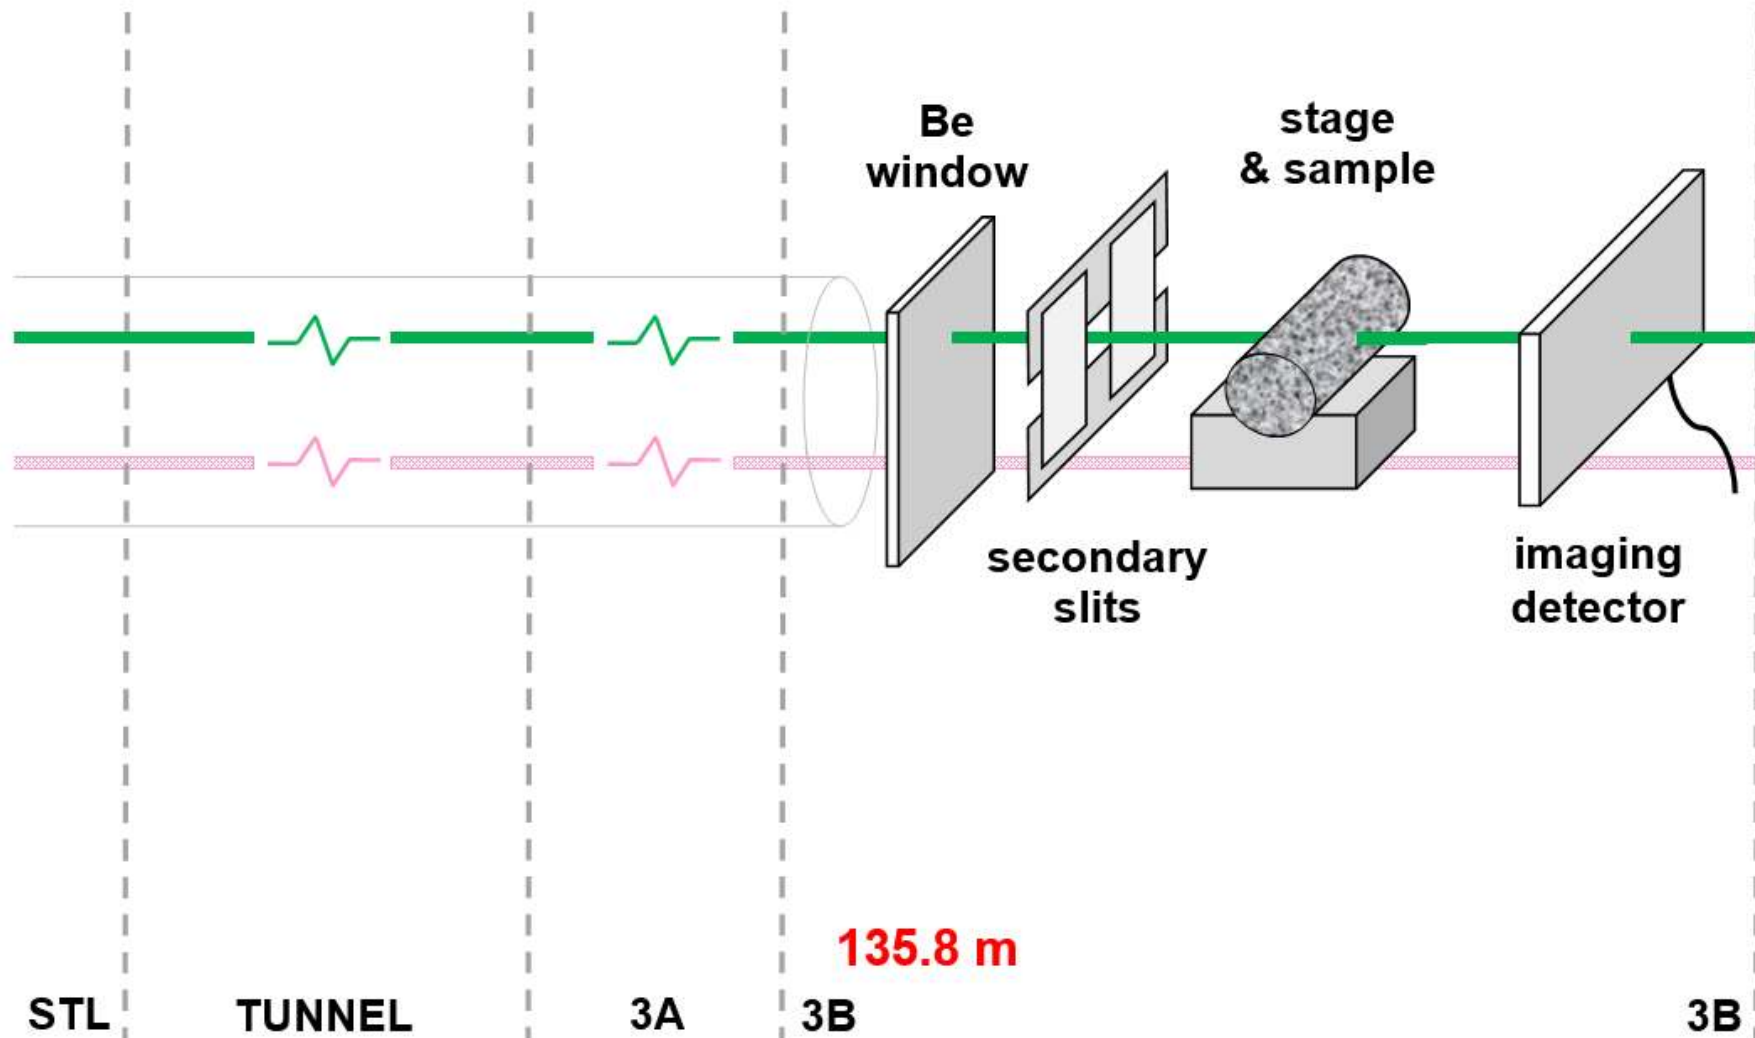

SCMPW



DCLM

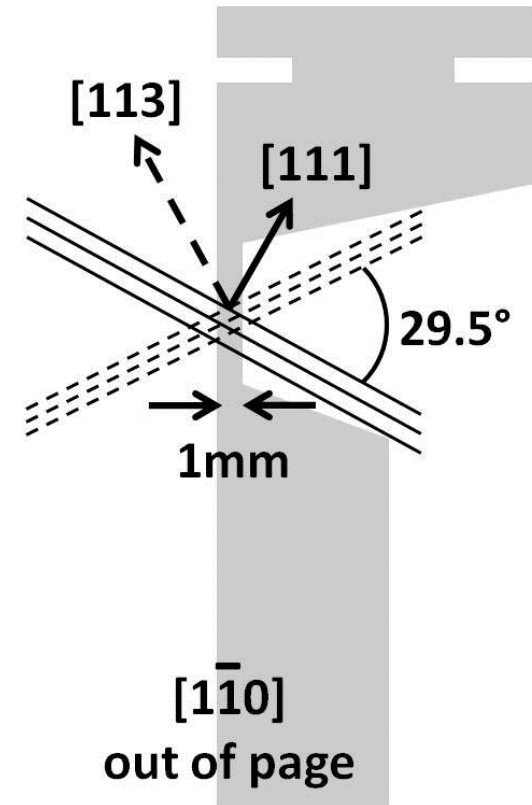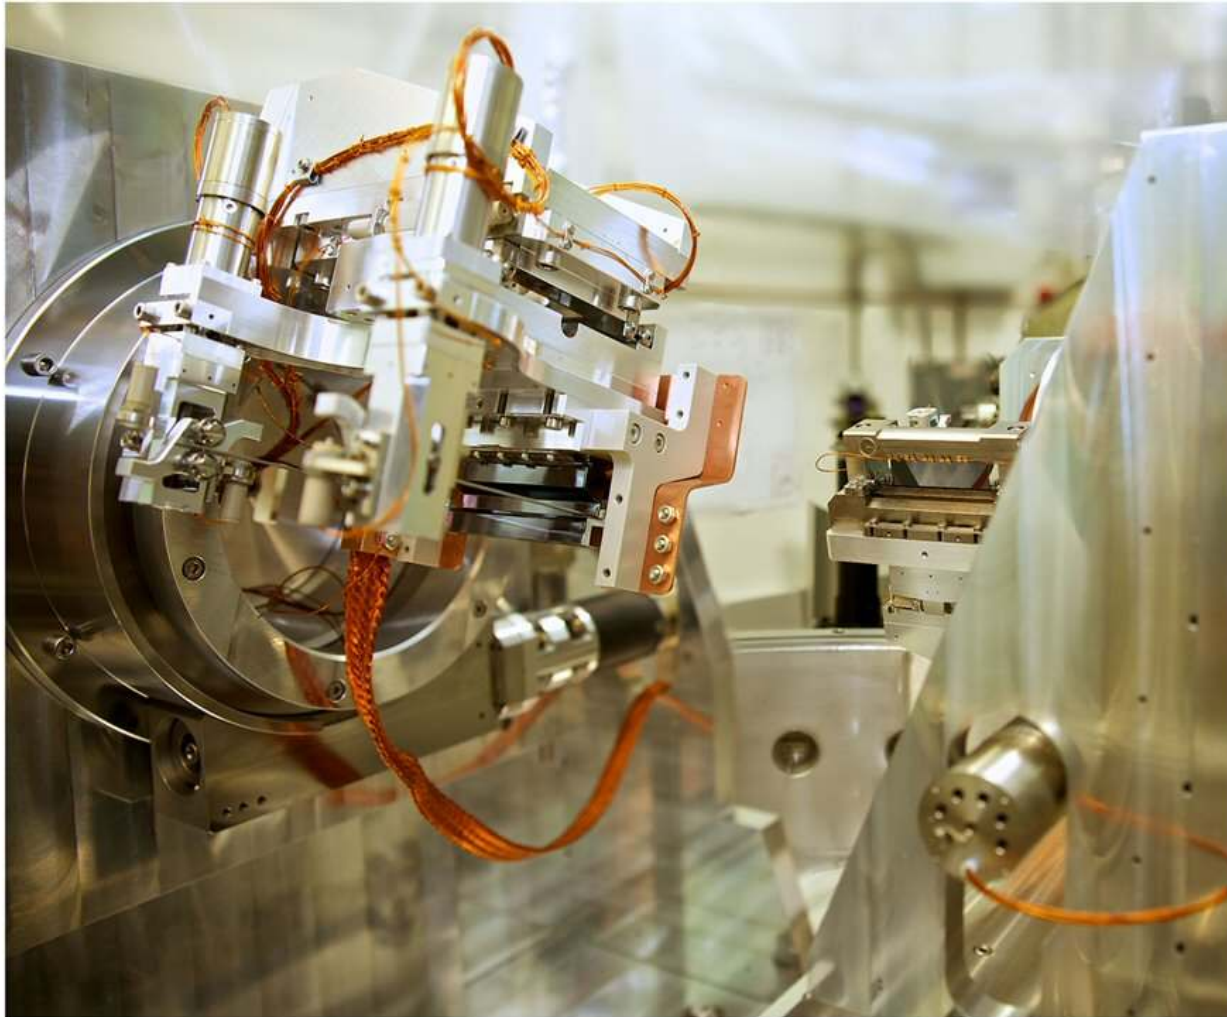


imaging detector details




detector	FOV (mm ²)	no. of pixels	pixel size (μm)	max. full fps	likely use
Diamond Optique Peter X-ray microscope with PCO.edge sensor	min: 1.66 x 1.40	2560 x 2160	0.64	50	high resolution imaging & CT of small objects
	max: 13.46 x 11.36	2560 x 2160	5.3	50	
Amethyst Scint-X DXI-11000	36.18 x 24.12	4024 x 2680	9	3	medium resolution imaging at higher energies
Ruby Single PCO.edge sensor, lens coupled to scintillator	min: 16.25 x 13.72	2560 x 2160	6.35	50	medium resolution imaging & CT at fast frame rates
	max: 57.1 x 48.2	2560 x 2160	22.3	50	
Amber Photonic Science Dual VHR Imager	100.14 x 33.48	8769 x 2923	11.4	1.2	medium resolution, large area imaging
Quartz Hamamatsu C9252DK-14 flat panel imager	min: 243.2 x 100	2432 x 100	100	146	therapy sample positioning, fast frame imaging & CT
	max: 243.2 x 123.2	1216 x 616	200	30	
Opal Teledyne Dalsa, Argus Pan	current: 220 x 6.9	8160 x 256	27	7.8	wide, medium resolution, for high energy imaging
	future: 440 x 6.9	16320 x 256	27	7.8	
Mica modular version of Ruby (In development)	min: 380 x 32.4	25600 x 2160	15	50	very large area, medium resolution imaging & CT
	max: 760 x 64.8	25600 x 2160	30	50	

detectors

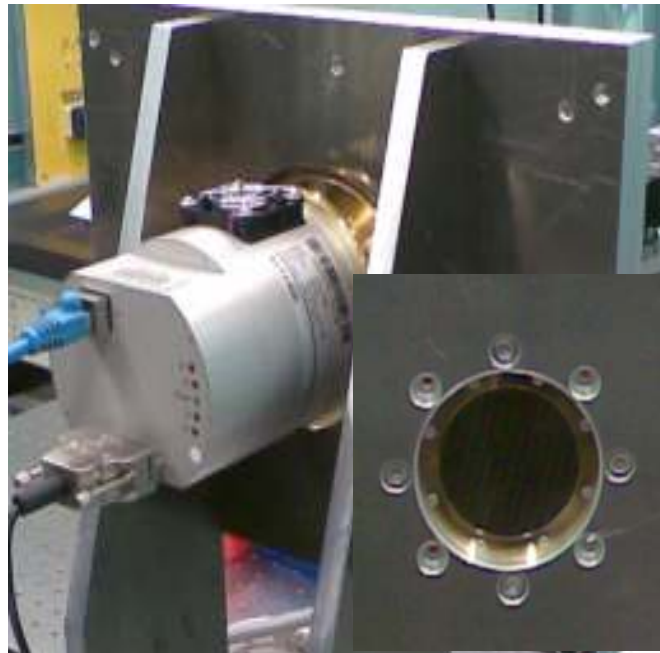

Amethyst – CsI

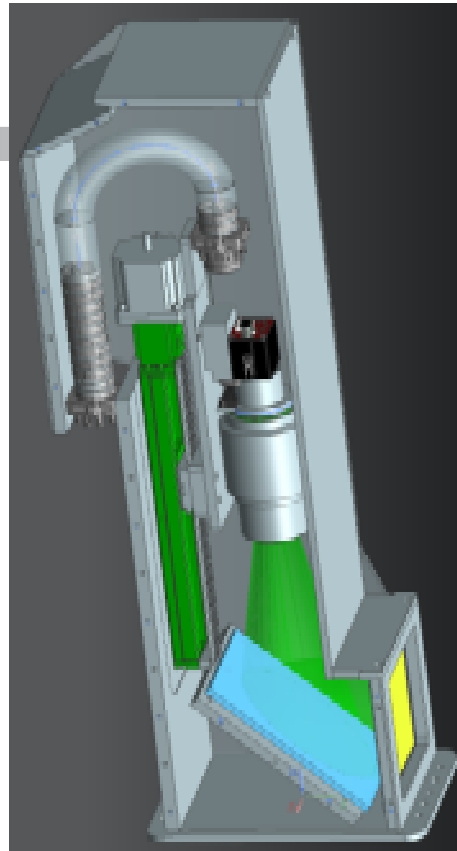

Ruby



Diamond

Amber – Dual CCD Gadox




Flat-panel CMOS imager – CsI

3B for imaging/ tomography users



“roll-off” – vertical direction

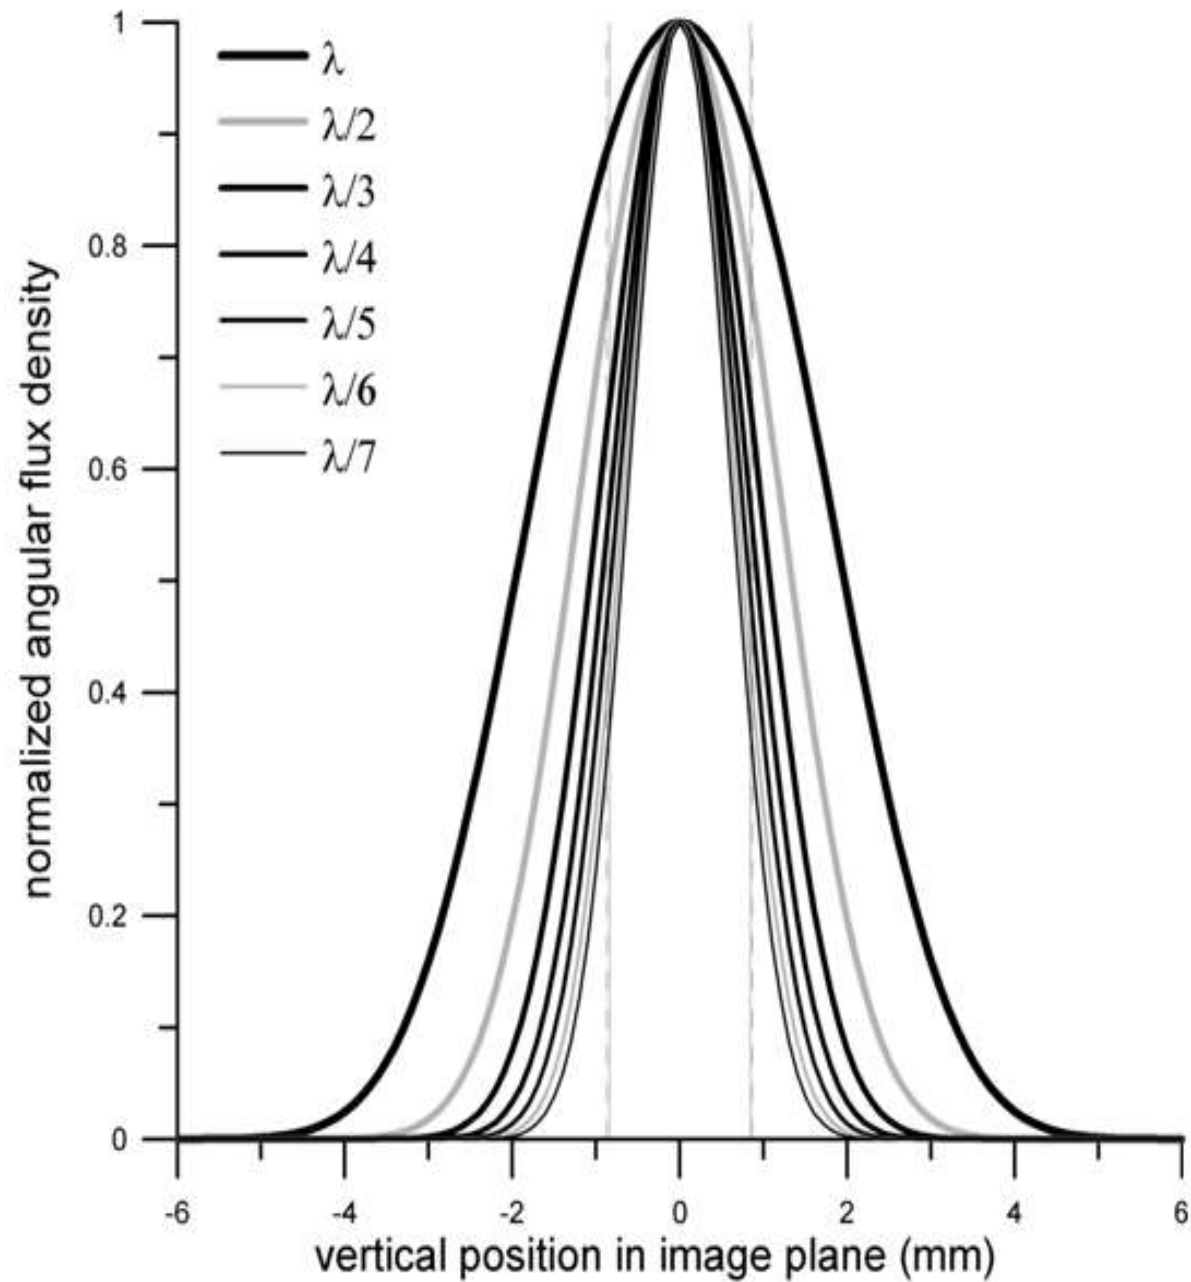



(a)



(b)



(c)




(d)

(a) 12.66 keV


(b) 18.00 keV

(c) 25.52 keV

(d) 30.49 keV

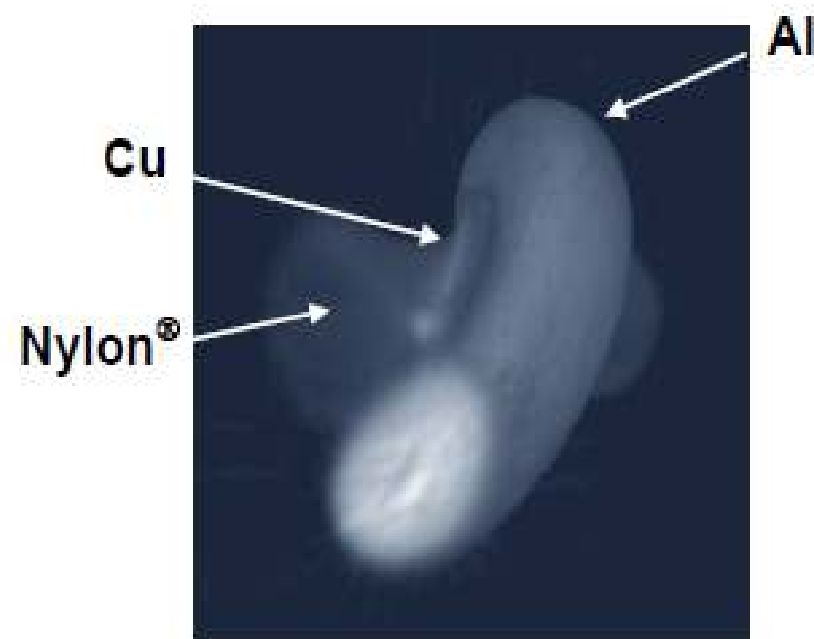

volume-rendered 12.66keV data

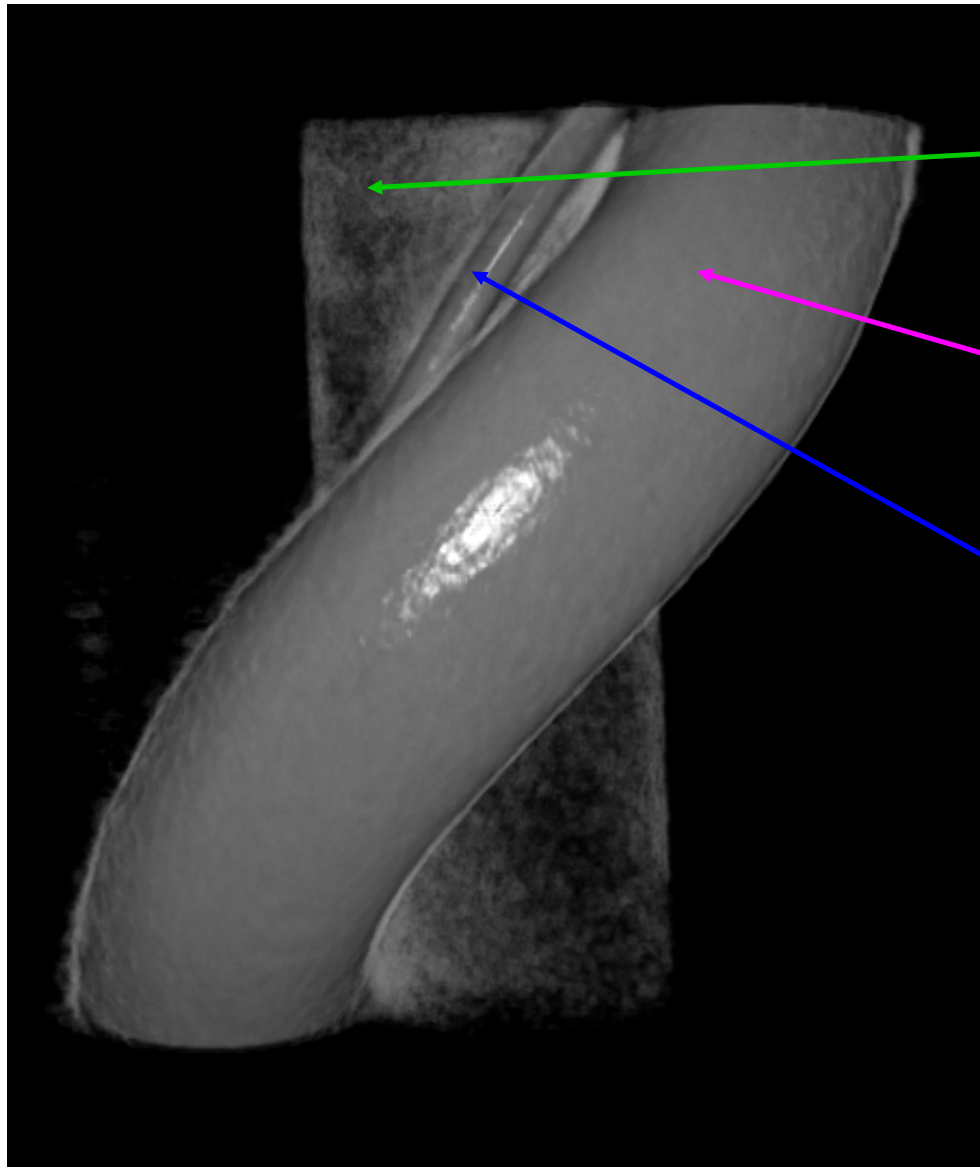

Nylon


Al

Cu


cross-section of human femur - data collected at ESRF in Grenoble, France



smallest features are osteocytes (of order $5\mu\text{m}$)

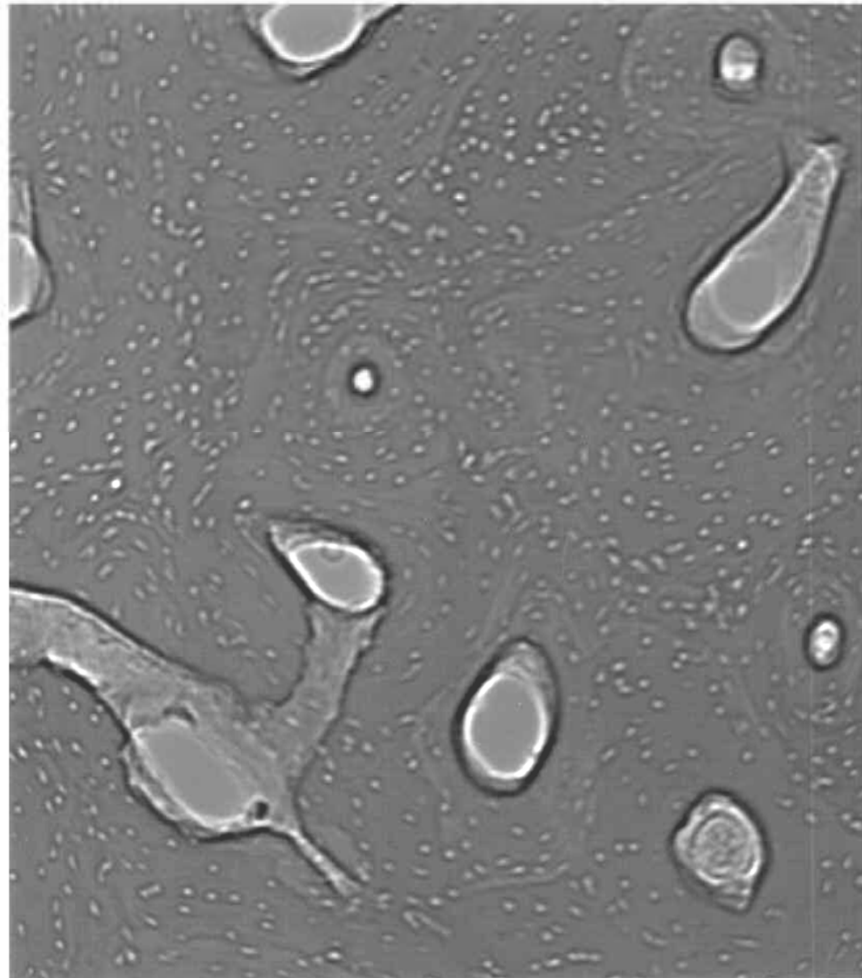


central section of a feather

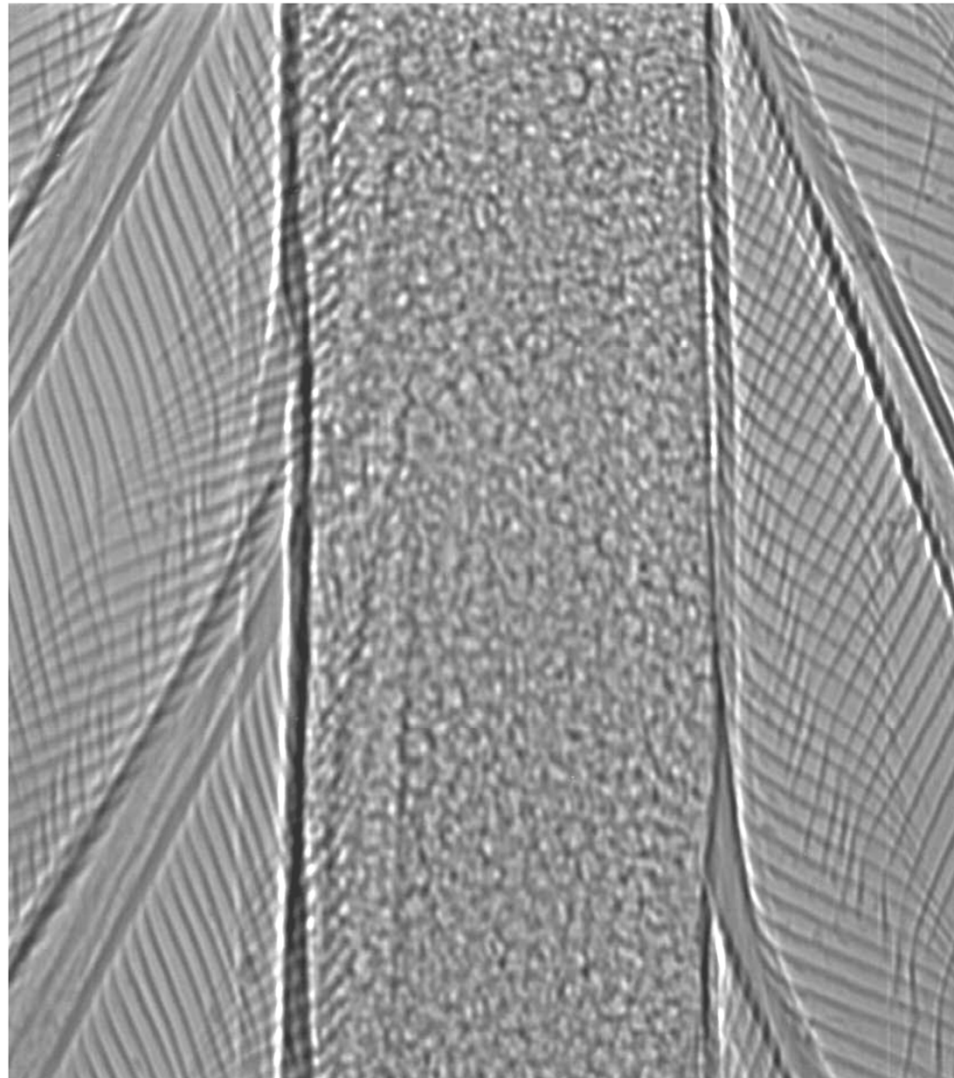


Graphite fibres ($\sim 10\mu\text{m}$) in Aluminium


- data collected at ESRF

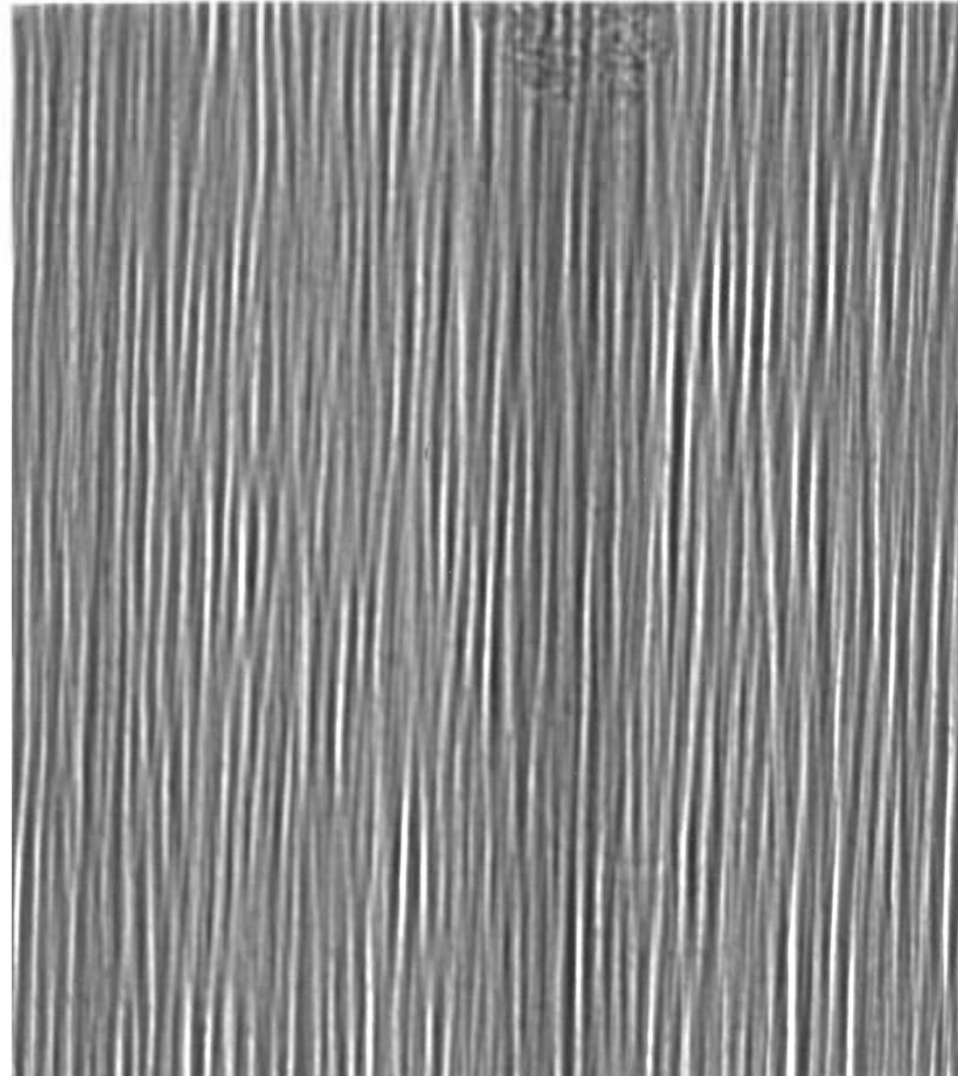

first X-ray images from IMBL (polychromatic) - December, 2008

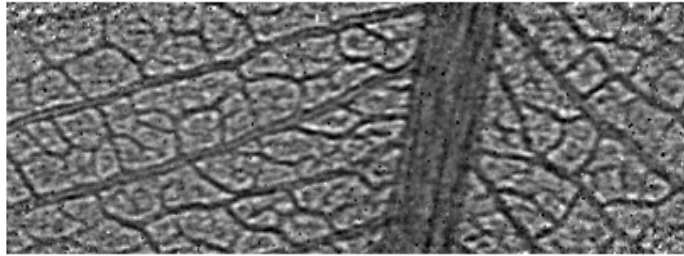


(a)


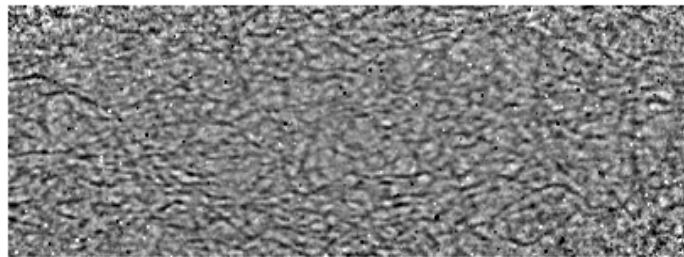


(b)

← ~6.2 mm →


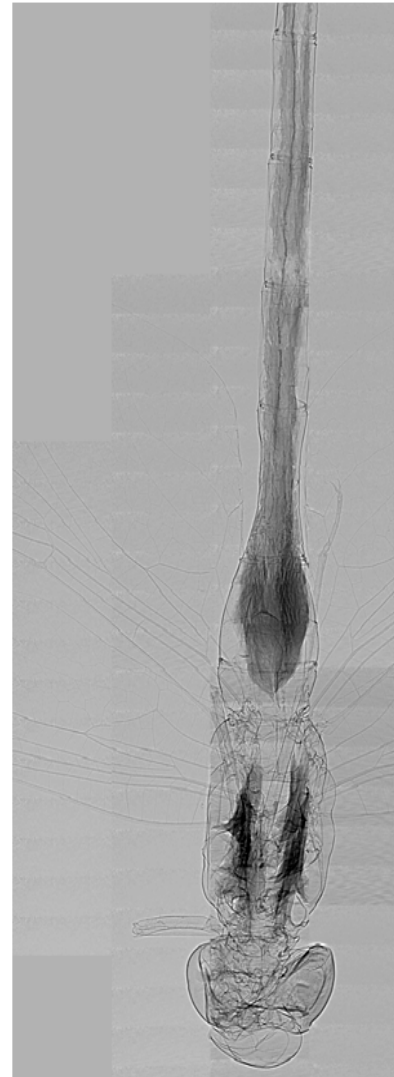


← ~26.5 mm →

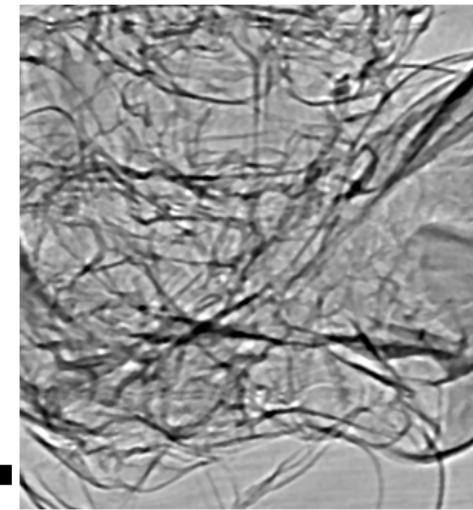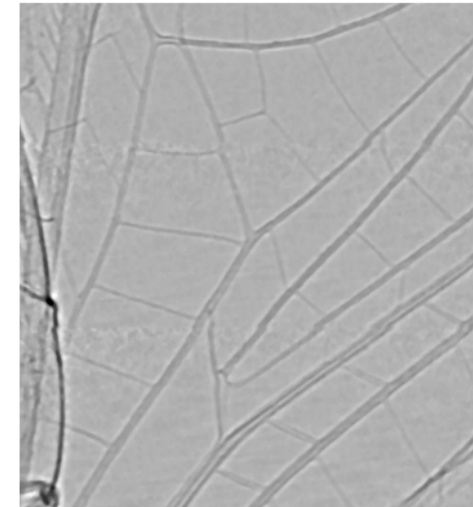

← ~6.5 mm →

first X-ray images from IMBL - mouse tibiae (different treatments & distances)

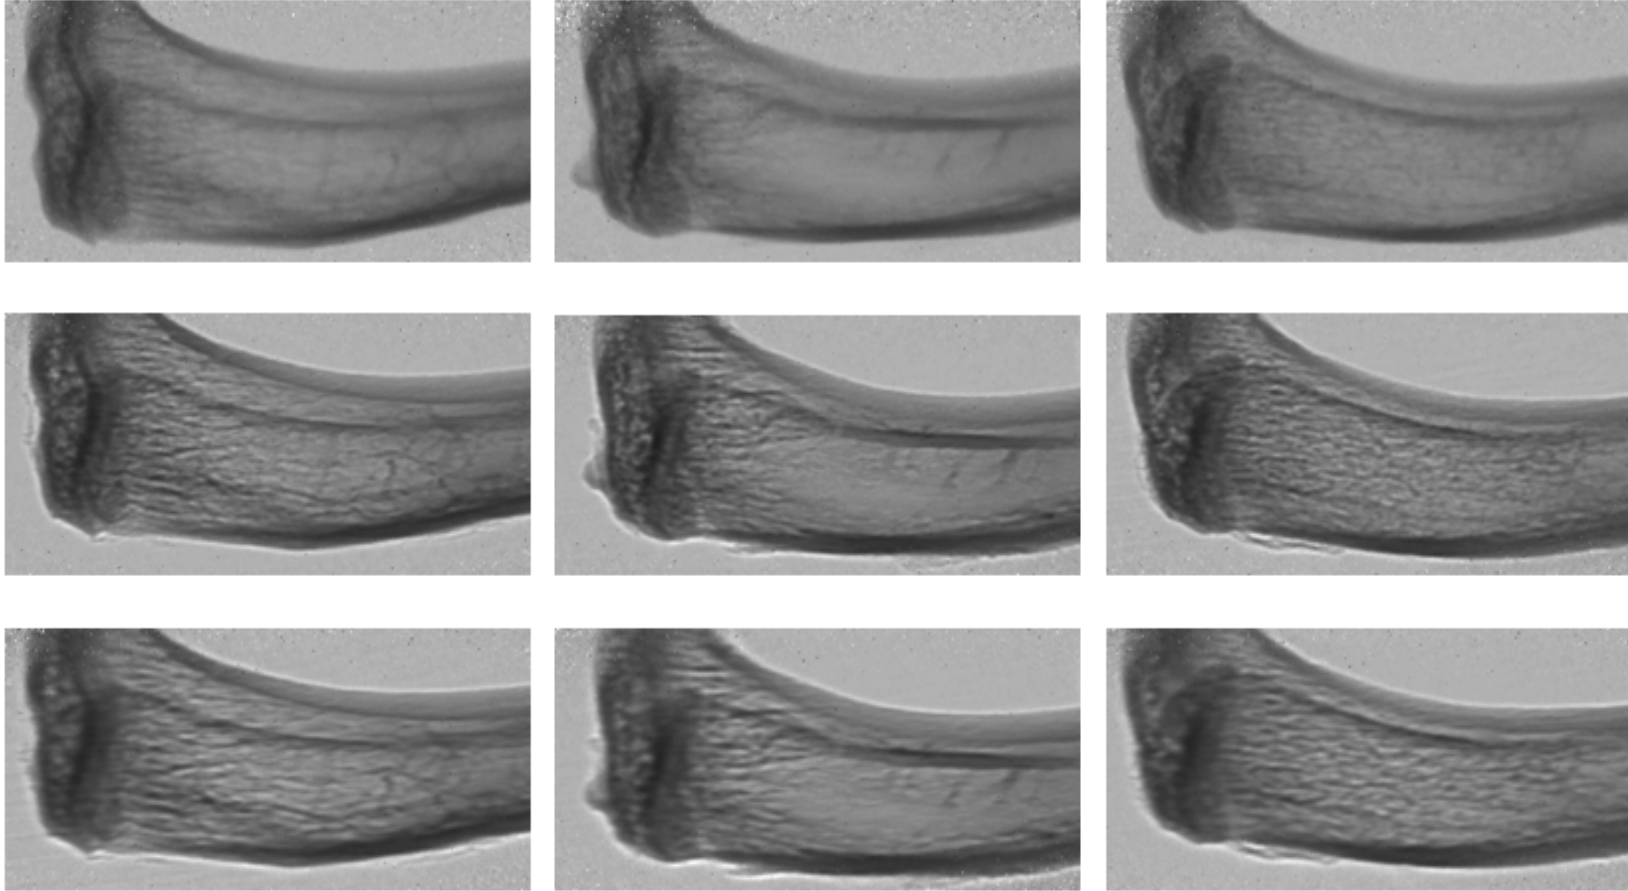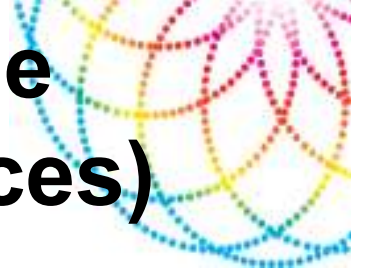


←~6.3 mm→

reconstructed tomography slices for leptin-treated mouse tibia



(d)

←~3.8mm→

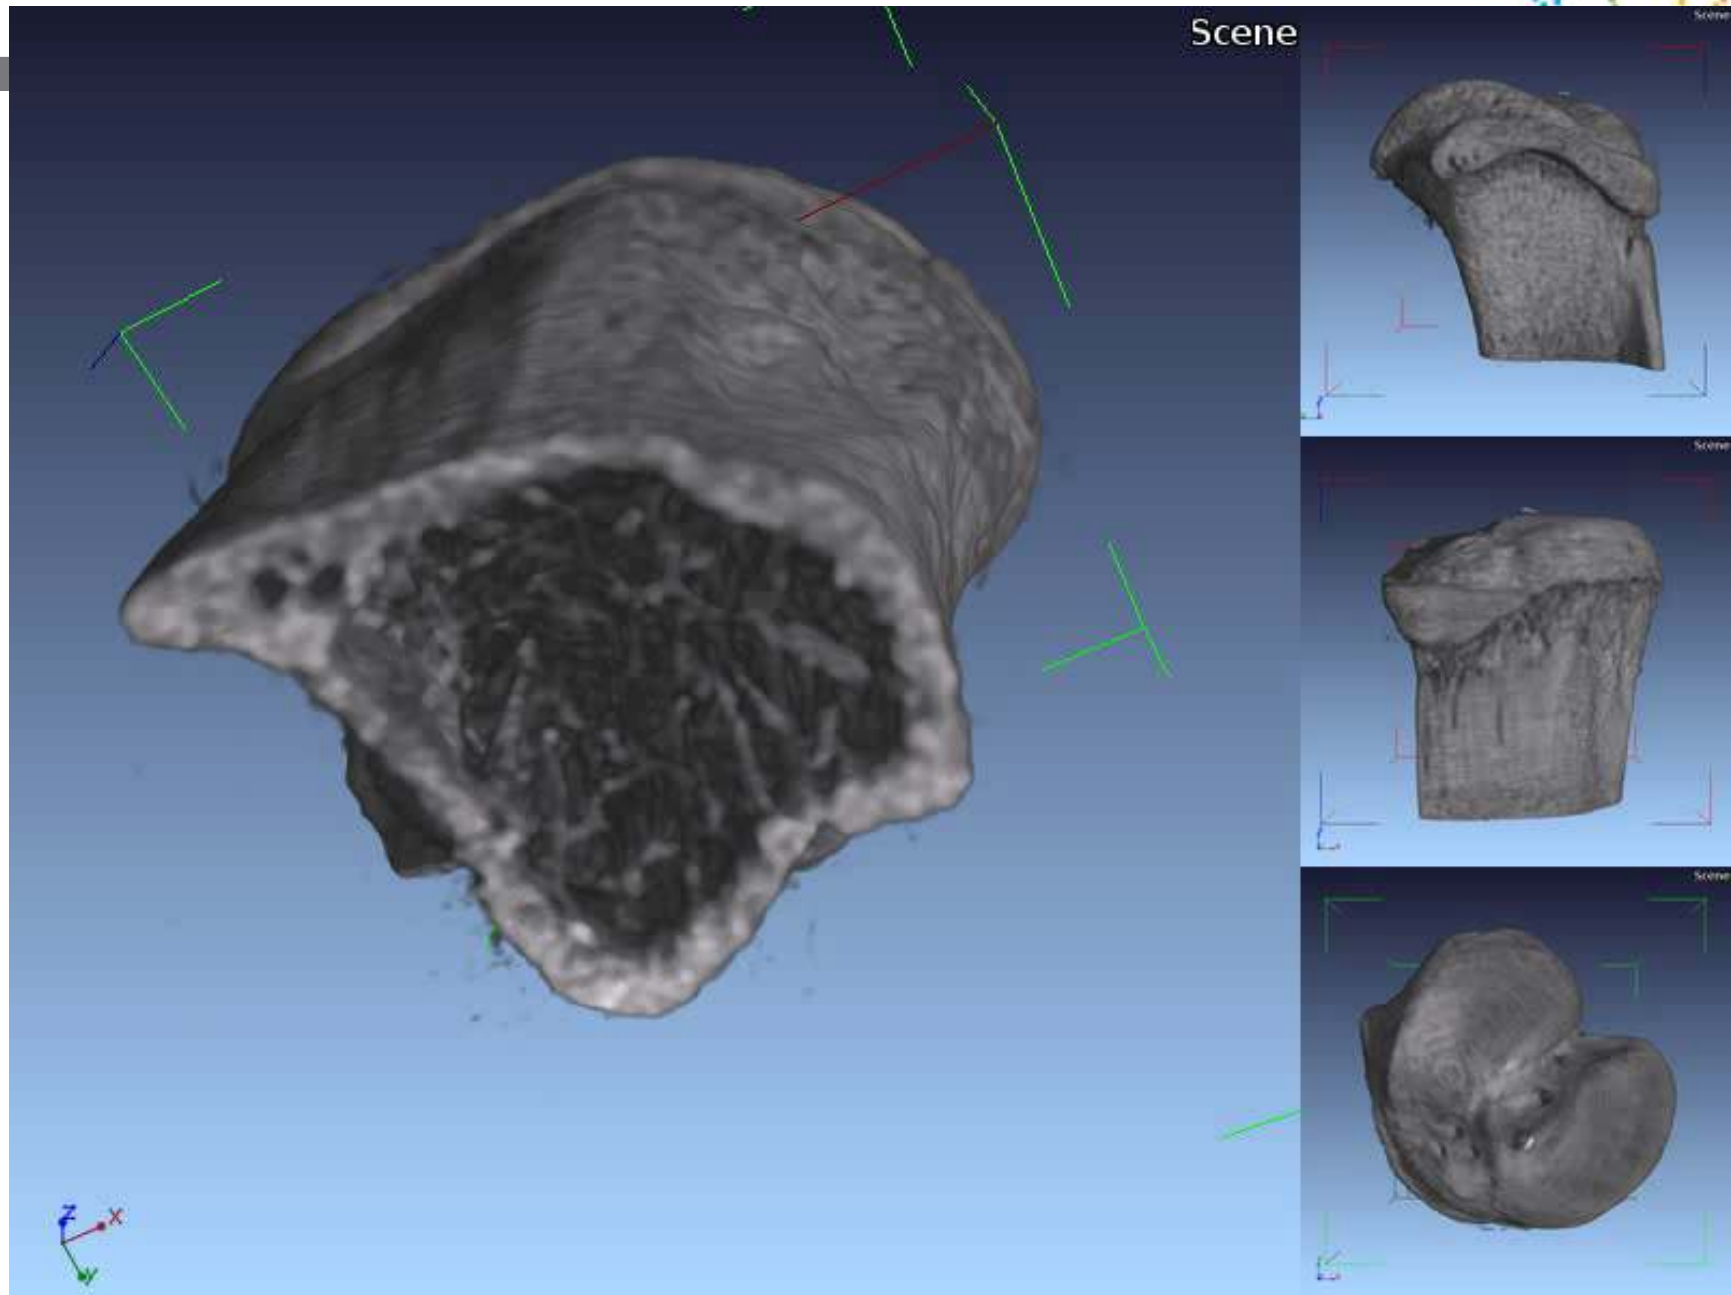



CSIRO Manufacturing/ IMBL, Australian Synchrotron

Dr Andrew Stevenson

Phone: +61 3 9518 5945

Email: andrew.stevenson@csiro.au

or andrew.stevenson@synchrotron.org.au

Thank you for your attention



Australian Synchrotron





“25keV.avi”, “50keV.avi” & “100keV.avi”

- **1024 μm $\times$ 1024 μm**
- **Cu**
- **$R_1 = 21 \text{ m}$ & $R_2 = 1 \text{ cm}$**
- **$\sigma_d = 6.3 \text{ } \mu\text{m}$**



“detector_resolution.avi”

- **1024 μm $\times$ 1024 μm**
- **Ge 0.5 mm**
- **$R_1 = 21 \text{ m}$ & $R_2 = 1 \text{ cm}$**
- **50 keV**



“signal_to_noise.avi”

- **1024 μm $\times$ 1024 μm**
- **Ge 0.5 mm**
- **$R_1 = 21 \text{ m}$ & $R_2 = 1 \text{ cm}$**
- **$\sigma_d = 5 \mu\text{m}$**
- **50 keV**



“Z.avi”

- **$1024\ \mu\text{m} \times 1024\ \mu\text{m}$**
- **$0.5\ \text{mm}$**
- **$R_1 = 21\ \text{m} \ \& \ R_2 = 1\ \text{cm}$**
- **$\sigma_d = 6.3\ \mu\text{m}$**
- **$50\ \text{keV}$**



“K_abs_edge.avi”

- **1024 μm $\times$ 1024 μm**
- **I (“IM”) & Ba (“BL”) 0.1 mm**
- **$R_1 = 21 \text{ m}$ & $R_2 = 1 \text{ cm}$**
- **$\sigma_d = 6.3 \mu\text{m}$**



“1B_PC.avi”, “2B_PC.avi” & “3B_PC.avi”

- **1024 μm $\times$ 1024 μm**
- **Al 0.1 mm**
- **$R_1 = 20$ m (1B), 34 m (2B) & 138 m (3B)**
- **$\sigma_d = 5$ μm , $\sigma_{s,h} = 320$ μm & $\sigma_{s,v} = 16$ μm**
- **25 keV**